
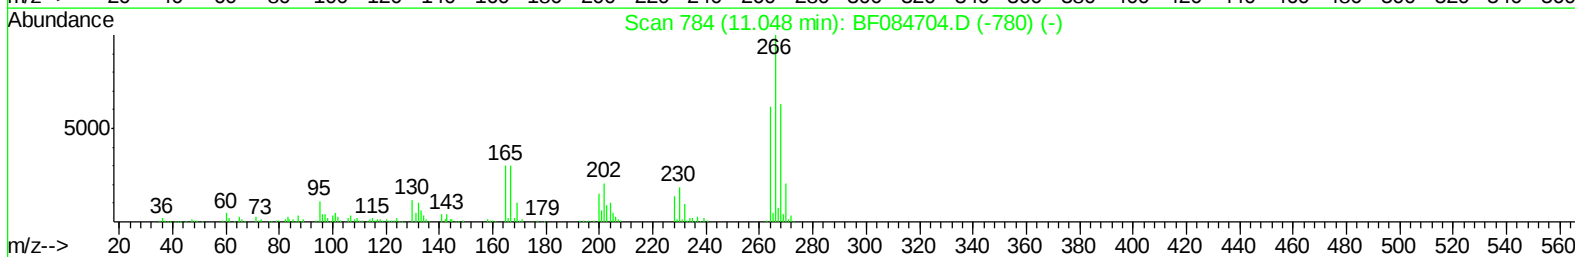
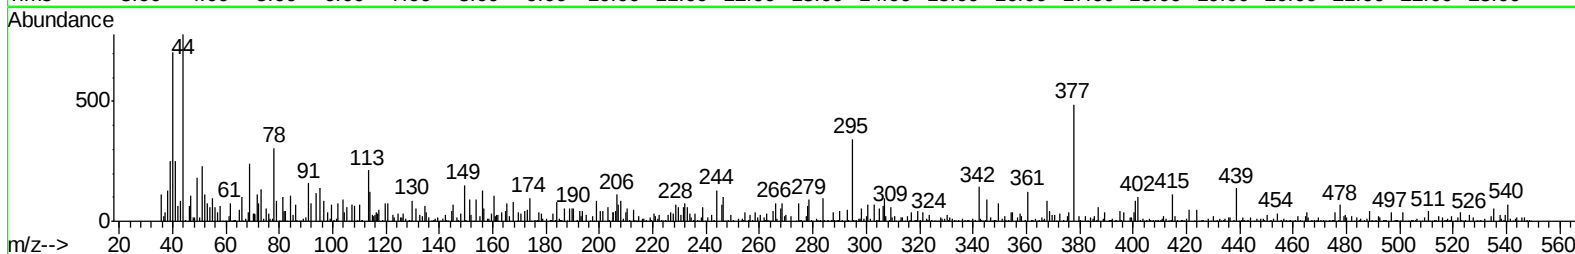


Data Path : Z:\HPCHEM1\BNA_E\Data\Be020416\
Data File : BE091385.D
Acq On : 4 Feb 2016 7:39
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 06:24:38 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

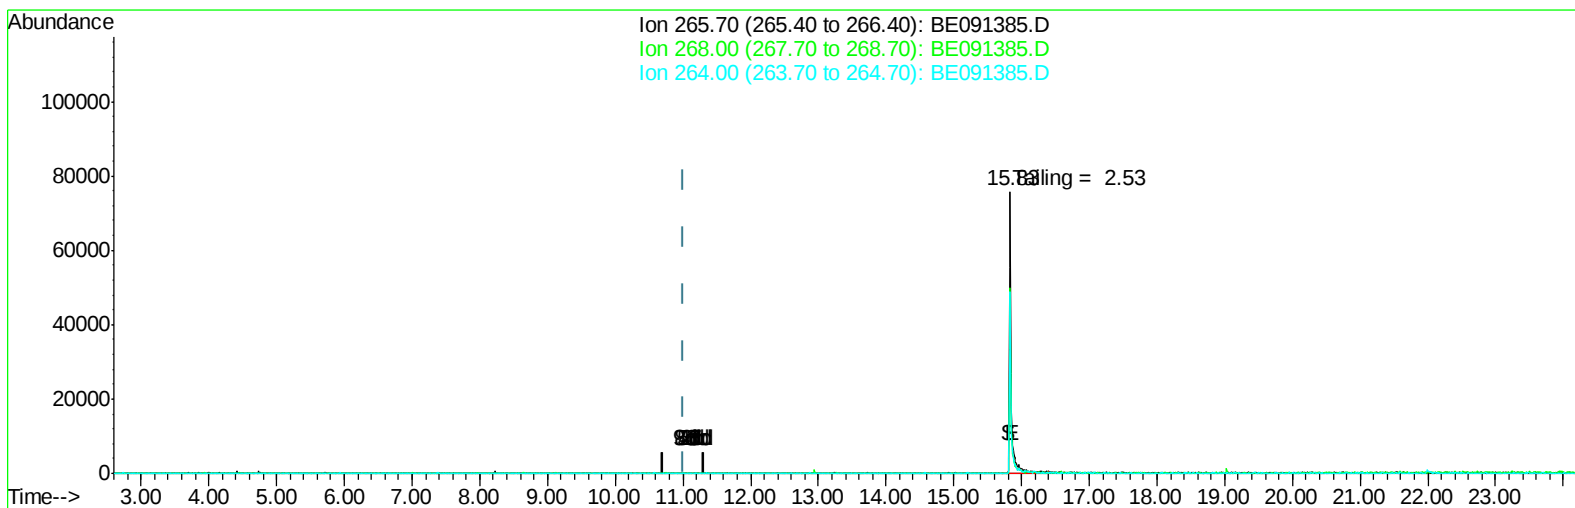

TIC: BE091385.D

(69) Pentachlorophenol (C)




11.187min (+0.173) 147.34ng

response 30

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	166.23#
264.00	62.70	5.19#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\Be020416\
Data File : BE091385.D
Acq On : 4 Feb 2016 7:39
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 06:24:38 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

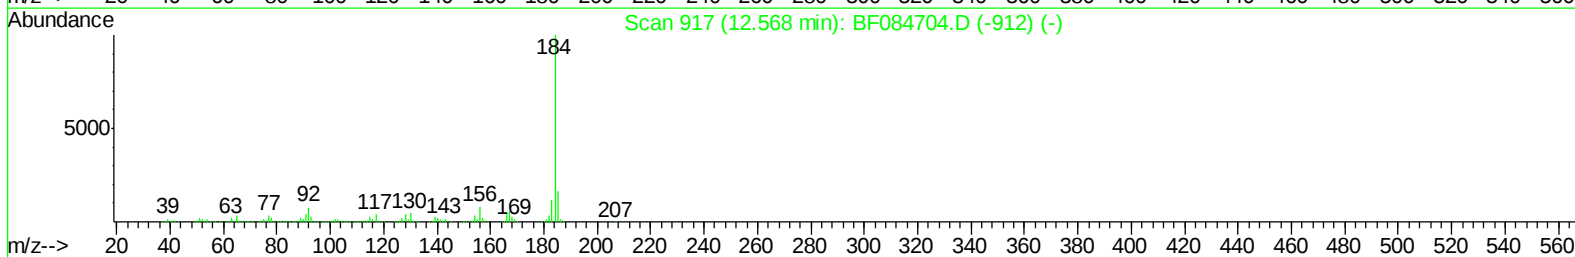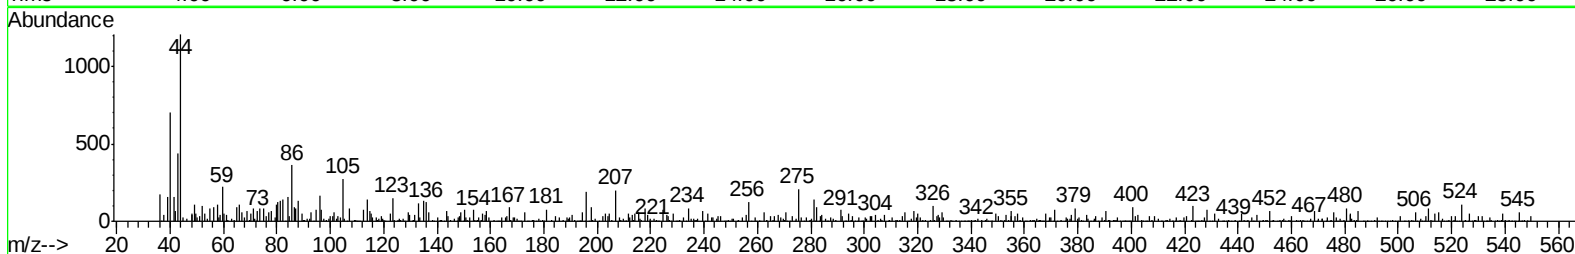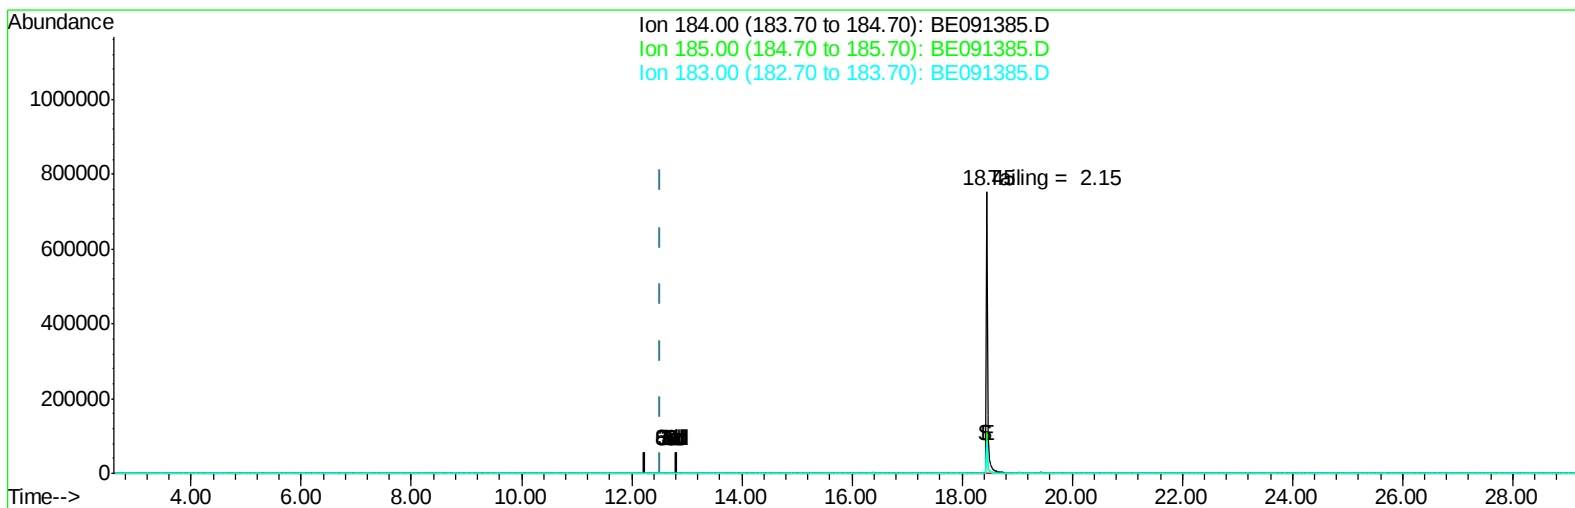

TIC: BE091385.D

(76) Benzidine

12.720min (+0.175) 24.68ng

response 22

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	78.79#
183.00	12.30	36.36#
0.00	0.00	0.00