


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020416\
 Data File : BE091385.D
 Acq On : 4 Feb 2016 7:39
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 03 00:27:53 2016

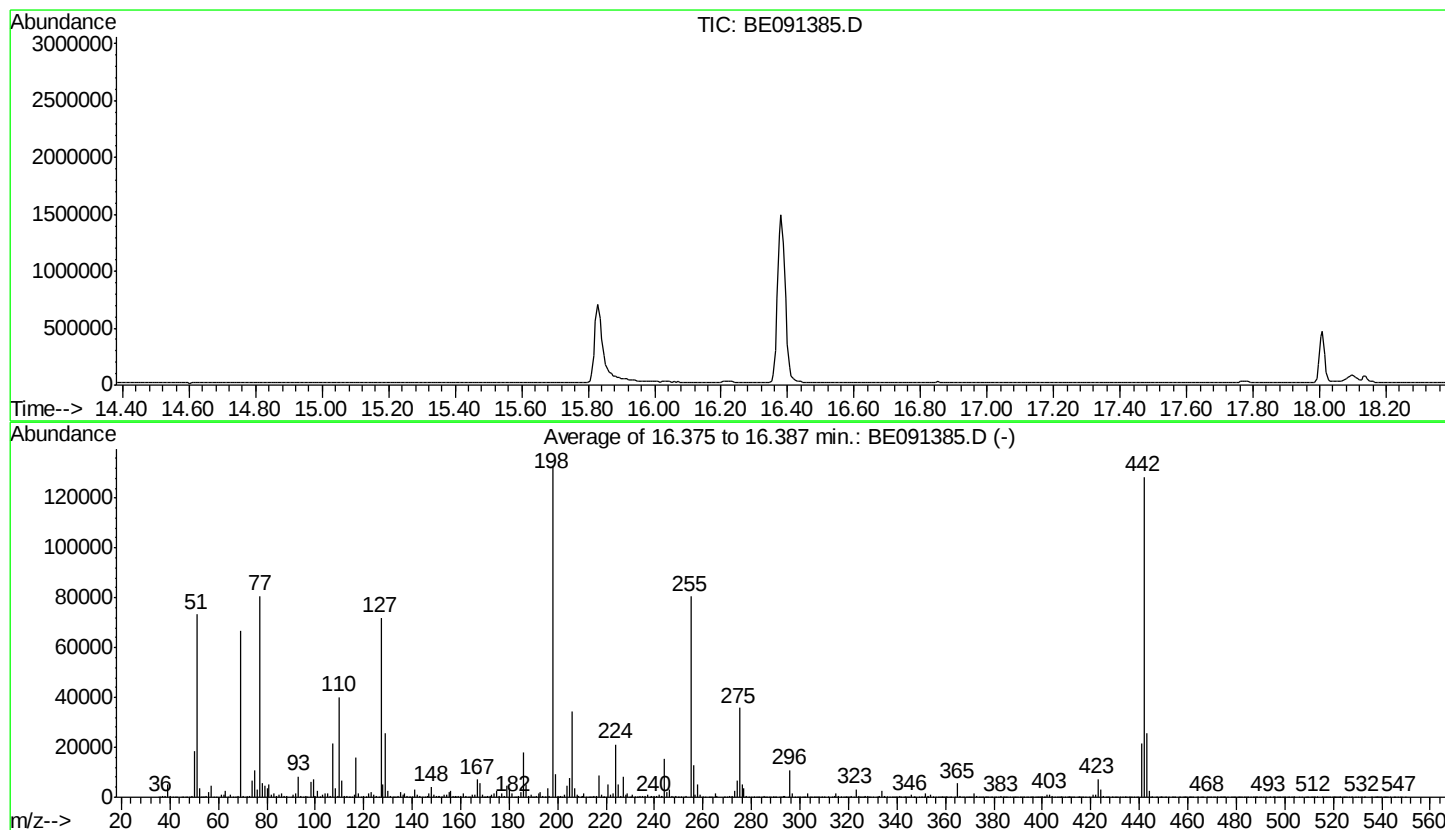

AutoFind: Scans 2346, 2347, 2348; Background Corrected with Scan 2333

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.0	73207	PASS
68	69	0.00	2	1.0	675	PASS
69	198	0.00	100	50.1	66637	PASS
70	69	0.00	2	0.4	280	PASS
127	198	10	80	54.1	72010	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	132999	PASS
199	198	5	9	6.9	9180	PASS
275	198	10	60	26.8	35705	PASS
365	198	1	100	4.2	5575	PASS
441	442	0.01	24	16.7	21528	PASS
442	198	50	100	96.7	128606	PASS
443	442	15	24	19.9	25574	PASS