


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE020515\
 Data File : BE089499.D
 Acq On : 5 Feb 2015 10:31
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE020515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 06 03:21:38 2015

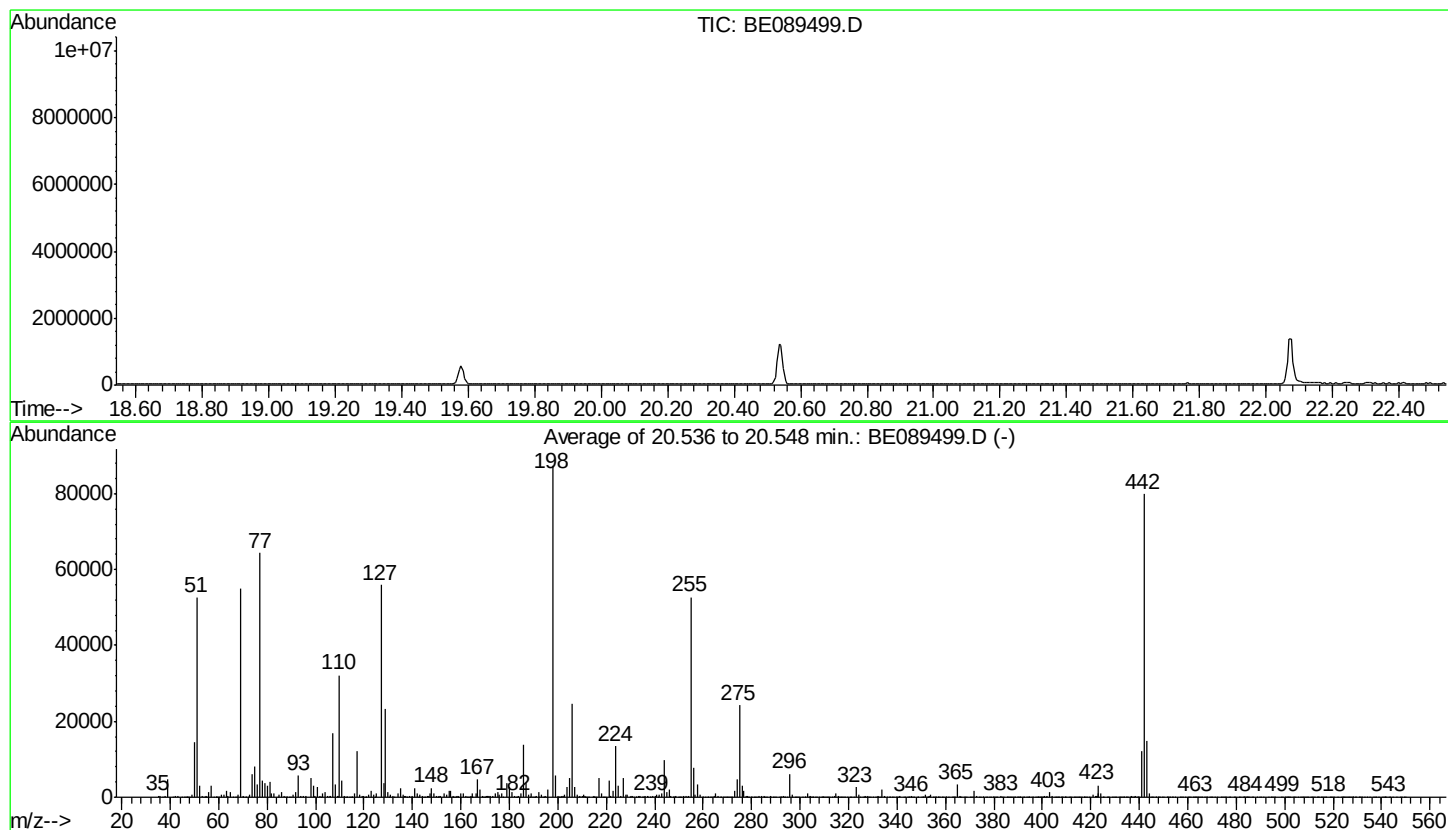

AutoFind: Scans 3259, 3260, 3261; Background Corrected with Scan 3252

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.2	52612	PASS
68	69	0.00	2	1.1	604	PASS
69	198	0.00	100	62.7	54821	PASS
70	69	0.00	2	0.4	197	PASS
127	198	10	80	64.0	55924	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87370	PASS
199	198	5	9	6.7	5820	PASS
275	198	10	60	27.7	24171	PASS
365	198	1	100	3.8	3355	PASS
441	442	0.01	24	15.0	11986	PASS
442	198	50	100	91.5	79926	PASS
443	442	15	24	18.6	14877	PASS