

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020515\
 Data File : BE089503.D
 Acq On : 5 Feb 2015 13:18
 Operator : TP/IZ
 Sample : SSTDICCC001
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTDICCC001

Quant Time: Feb 06 02:49:07 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SIMPAH-BE020515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 06 02:40:17 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.49	152	31396	5.00	ng	0.00
2) Naphthalene-d8	12.40	136	132520	5.00	ng	0.00
6) Acenaphthene-d10	16.59	164	65560	5.00	ng	0.00
11) Phenanthrene-d10	19.90	188	128634	5.00	ng	0.00
16) Chrysene-d12	23.76	240	143431	5.00	ng	0.00
22) Perylene-d12	25.46	264	145552	5.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) Nitrobenzene-d5	10.76	82	10361	1.02	ng	0.00
7) 2-Fluorobiphenyl	15.03	172	23554	1.14	ng	0.00
18) Terphenyl-d14	22.40	244	29874	1.20	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
4) Naphthalene	12.45	128	34641	1.04	ng	100
5) 2-Methylnaphthalene	14.11	142	25028	1.15	ng	100
8) Acenaphthylene	16.24	152	166466	1.18	ng	100
9) Acenaphthene	16.65	154	25298	1.17	ng	100
10) Fluorene	17.90	166	29308	1.22	ng	100
12) Pentachlorophenol	19.58	266	317	0.25	ng	100
13) Phenanthrene	19.94	178	46246	1.18	ng	100
14) Anthracene	20.04	178	42845	1.23	ng	100
15) Fluoranthene	21.84	202	46146	1.24	ng	100
17) Pyrene	22.15	202	49120	1.20	ng	100
19) Benzo(a)anthracene	23.75	228	190352	1.21	ng	100
20) Chrysene	23.79	228	193892	1.20	ng	100
21) Indeno(1,2,3-cd)pyrene	26.93	276	223160	1.33	ng	100
23) Benzo(b)fluoranthene	25.02	252	41159	1.22	ng	100
24) Benzo(k)fluoranthene	25.05	252	55685	1.20	ng	100
25) Benzo(a)pyrene	25.39	252	42142	1.23	ng	100
26) Dibenzo(a,h)anthracene	26.95	278	47343	1.29	ng	100
27) Benzo(a,h,i)perylene	27.36	276	186516	1.25	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020515\
Data File : BE089503.D
Acq On : 5 Feb 2015 13:18
Operator : TP/IZ
Sample : SSTDICCC001
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
LabSampleId :
SSTDICCC001

Quant Time: Feb 06 02:49:07 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SIMPAH-BE020515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 06 02:40:17 2015
Response via : Initial Calibration





#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 9.49 min Scan# 1513

Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18

Instrument :

BNA_E

LabSampleId :

SSTDICCC001


Tot Ion:152 Resp: 31396

Ion Ratio Lower Upper

152 100

150 156.3 125.0 187.6




115 70.8 56.6 85.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E



#2

Naphthalene-d8

Concen: 5.00 ng

RT: 12.40 min Scan# 2351

Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18


Tgt Ion:136 Resp: 132520

Ion Ratio Lower Upper

136 100

137 10.7 8.6 12.8



54 7.5 6.0 9.0




Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0



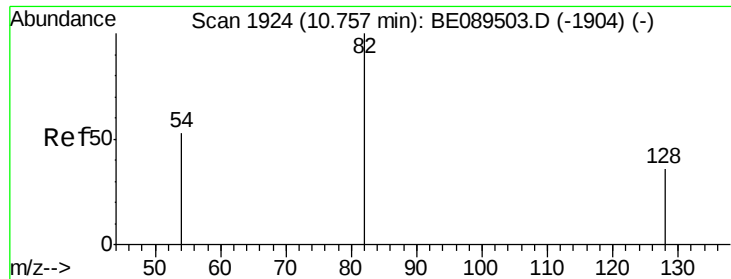

#3

Nitrobenzene-d5

Concen: 1.02 ng

RT: 10.76 min Scan# 1924

Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18

Instrument :

BNA_E

LabSampleId :

SSTDICCC001


Tot Ion: 82 Resp: 10361

Ion Ratio Lower Upper

82 100

128 36.6 29.3 43.9

54 53.3 42.6 64.0



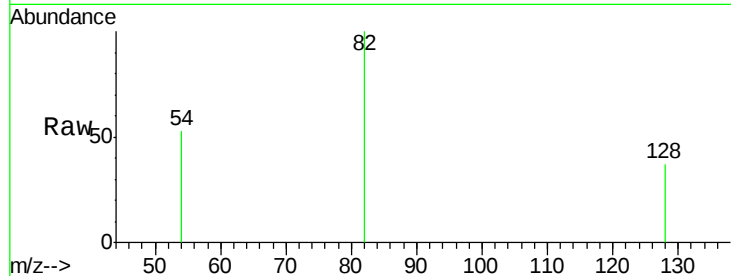


Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

Time-->



#4

Naphthalene

Concen: 1.04 ng

RT: 12.45 min Scan# 2360

Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18


Tgt Ion: 128 Resp: 34641

Ion Ratio Lower Upper

128 100

129 11.0 8.8 13.2

127 12.9 10.3 15.5





Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

Time-->





#5

2-Methylnaphthalene

Concen: 1.15 ng

RT: 14.11 min Scan# 2694

Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18

Instrument :

BNA_E

LabSampleId :

SSTDICCC001





Tot Ion:142 Resp: 25028

Ion Ratio Lower Upper

142 100

141 82.9 66.3 99.5

115 38.9 31.1 46.7



#6

Acenaphthene-d10

Concen: 5.00 ng

RT: 16.59 min Scan# 3096

Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18




Tgt Ion:164 Resp: 65560

Ion Ratio Lower Upper

164 100

162 95.8 76.6 115.0

160 43.3 34.6 52.0





#7

2-Fluorobiphenyl

Concen: 1.14 ng

RT: 15.03 min Scan# 2897

Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18

Instrument :

BNA_E

LabSampleId :

SSTDICCC001


Tot Ion:172 Resp: 23554

Ion Ratio Lower Upper

172 100

171 34.2 27.4 41.0




170 23.0 18.4 27.6



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

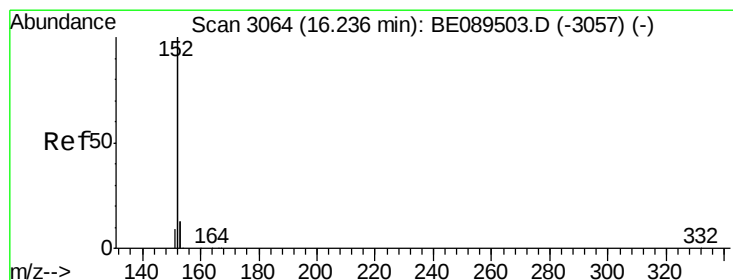

#8

Acenaphthylene

Concen: 1.18 ng

RT: 16.24 min Scan# 3064

Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18


Tgt Ion:152 Resp: 166466

Ion Ratio Lower Upper

152 100

151 4.9 3.9 5.9



153 13.0 10.4 15.6




Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E





#9

Acenaphthene

Concen: 1.17 ng

RT: 16.65 min Scan# 3102

Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18

Instrument :


BNA_E

LabSampleId :

SSTDICCC001

Tot Ion:154 Resp: 25298

Ion	Ratio	Lower	Upper
154	100		
153	426.9	341.5	512.3
152	208.2	166.6	249.8



Abundance




Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

16.65

Time-->



#10

Fluorene

Concen: 1.22 ng

RT: 17.90 min Scan# 3216


Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18

Tgt Ion:166 Resp: 29308

Ion	Ratio	Lower	Upper
166	100		
165	92.0	73.6	110.4
167	13.2	10.6	15.8



Abundance



Ion 166.00 (165.70 to 166.70): E


Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

17.90

Time-->









#11
Phenanthrene-d10
Concen: 5.00 ng
RT: 19.90 min Scan# 3415
Delta R.T. 0.00 min
Lab File: BE089503.D
Acq: 5 Feb 2015 13:18




Instrument :
BNA_E
LabSampleId :
SSTDICCC001


Tot Ion:188 Resp: 128634
Ion Ratio Lower Upper
188 100
94 10.3 8.2 12.4
80 10.9 8.7 13.1



#12
Pentachlorophenol
Concen: 0.25 ng
RT: 19.58 min Scan# 3379
Delta R.T. 0.00 min
Lab File: BE089503.D
Acq: 5 Feb 2015 13:18

Tgt Ion:266 Resp: 317
Ion Ratio Lower Upper
266 100
268 70.9 56.7 85.1
264 64.9 51.9 77.9









#13
Phenanthrene
Concen: 1.18 ng
RT: 19.94 min Scan# 3419
Delta R.T. 0.00 min
Lab File: BE089503.D
Acq: 5 Feb 2015 13:18




Instrument :
BNA_E
LabSampleId :
SSTDICCC001


Tot Ion:178 Resp: 46246
Ion Ratio Lower Upper
178 100
176 19.2 15.4 23.0
179 15.5 12.4 18.6



#14
Anthracene
Concen: 1.23 ng
RT: 20.04 min Scan# 3430
Delta R.T. 0.00 min
Lab File: BE089503.D
Acq: 5 Feb 2015 13:18

Tgt Ion:178 Resp: 42845
Ion Ratio Lower Upper
178 100
176 18.3 14.6 22.0
179 15.1 12.1 18.1









#15
 Fluoranthene
 Concen: 1.24 ng
 RT: 21.84 min Scan# 3714
 Delta R.T. 0.00 min
 Lab File: BE089503.D
 Acq: 5 Feb 2015 13:18




Instrument :
 BNA_E
 LabSampleId :
 SSTDICC001


Tot Ion:202 Resp: 46146
 Ion Ratio Lower Upper
 202 100
 101 14.1 11.3 16.9
 203 17.2 13.8 20.6



#16
 Chrysene-d12
 Concen: 5.00 ng
 RT: 23.76 min Scan# 4046
 Delta R.T. 0.00 min
 Lab File: BE089503.D
 Acq: 5 Feb 2015 13:18

Tgt Ion:240 Resp: 143431
 Ion Ratio Lower Upper
 240 100
 120 12.0 9.6 14.4
 236 24.3 19.4 29.2





#17

Pvrene

Concen: 1.20 ng

RT: 22.15 min Scan# 3773

Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18

Instrument :

BNA_E

LabSampleId :

SSTDICCC001


Tot Ion:202 Resp: 49120

Ion Ratio Lower Upper

202 100

200 20.6 16.5 24.7




203 17.5 14.0 21.0



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E



#18

Terphenyl-d14

Concen: 1.20 ng

RT: 22.40 min Scan# 3821

Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18


Tgt Ion:244 Resp: 29874

Ion Ratio Lower Upper

244 100

212 6.9 5.5 8.3



122 13.9 11.1 16.7



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E





#19

Benzo(a)anthracene

Concen: 1.21 ng

RT: 23.75 min Scan# 4044

Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18

Instrument :

BNA_E

LabSampleId :

SSTDICCC001


Tot Ion:228 Resp: 190352

Ion Ratio Lower Upper


228 100

226 26.3 21.0 31.6



229 19.4 15.5 23.3



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E



Time-->



#20

Chrysene

Concen: 1.20 ng

RT: 23.79 min Scan# 4051

Delta R.T. 0.00 min

Lab File: BE089503.D

Acq: 5 Feb 2015 13:18


Tgt Ion:228 Resp: 193892

Ion Ratio Lower Upper


228 100

226 27.9 22.3 33.5


229 19.2 15.4 23.0




Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E



Time-->







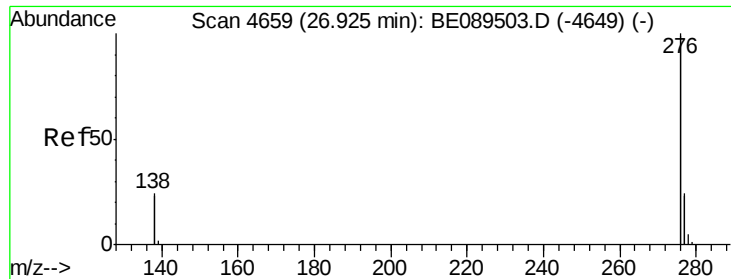

#21
 Indeno(1,2,3-cd)pyrene
 Concen: 1.33 ng
 RT: 26.93 min Scan# 4659
 Delta R.T. 0.00 min
 Lab File: BE089503.D
 Acq: 5 Feb 2015 13:18




Instrument :
 BNA_E
 LabSampleId :
 SSTDICC001

Tot Ion:276 Resp: 223160
 Ion Ratio Lower Upper
 276 100
 138 29.0 23.2 34.8
 277 24.7 19.8 29.6



#22
 Perylene-d12
 Concen: 5.00 ng
 RT: 25.46 min Scan# 4375
 Delta R.T. 0.00 min
 Lab File: BE089503.D
 Acq: 5 Feb 2015 13:18

Tgt Ion:264 Resp: 145552
 Ion Ratio Lower Upper
 264 100
 260 23.8 19.0 28.6
 265 21.3 17.0 25.6









#23
Benzo(b)fluoranthene
Concen: 1.22 ng
RT: 25.02 min Scan# 4278
Delta R.T. 0.00 min
Lab File: BE089503.D
Acq: 5 Feb 2015 13:18




Instrument :
BNA_E
LabSampleId :
SSTDICCC001

Tot Ion:252 Resp: 41159
Ion Ratio Lower Upper
252 100
253 21.7 17.4 26.0
125 12.0 9.6 14.4



#24
Benzo(k)fluoranthene
Concen: 1.20 ng
RT: 25.05 min Scan# 4284
Delta R.T. 0.00 min
Lab File: BE089503.D
Acq: 5 Feb 2015 13:18

Tgt Ion:252 Resp: 55685
Ion Ratio Lower Upper
252 100
253 21.3 17.0 25.6
125 12.8 10.2 15.4









#25
Benzo(a)pyrene
Concen: 1.23 ng
RT: 25.39 min Scan# 4360
Delta R.T. 0.00 min
Lab File: BE089503.D
Acq: 5 Feb 2015 13:18




Instrument :
BNA_E
LabSampleId :
SSTDICCC001

Tot Ion:252 Resp: 42142
Ion Ratio Lower Upper
252 100
253 22.2 17.8 26.6
125 13.4 10.7 16.1



#26
Dibenzo(a,h)anthracene
Concen: 1.29 ng
RT: 26.95 min Scan# 4663
Delta R.T. 0.00 min
Lab File: BE089503.D
Acq: 5 Feb 2015 13:18

Tgt Ion:278 Resp: 47343
Ion Ratio Lower Upper
278 100
139 18.3 14.6 22.0
279 23.7 19.0 28.4






#27
 Benzo(a,h,i)perylene
 Concen: 1.25 ng
 RT: 27.36 min Scan# 4725
 Delta R.T. 0.00 min
 Lab File: BE089503.D
 Acq: 5 Feb 2015 13:18

Instrument :
 BNA_E
 LabSampleId :
 SSTDICC001

Tot Ion	Ratio	Lower	Upper
276	100		
277	23.3	18.6	28.0
138	26.0	20.8	31.2



Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

