


Data Path : Z:\HPCHEM1\BNA E\Data\BE020515\
 Data File : BE089516.D
 Acq On : 5 Feb 2015 23:27
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE020515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 06 12:30:39 2015

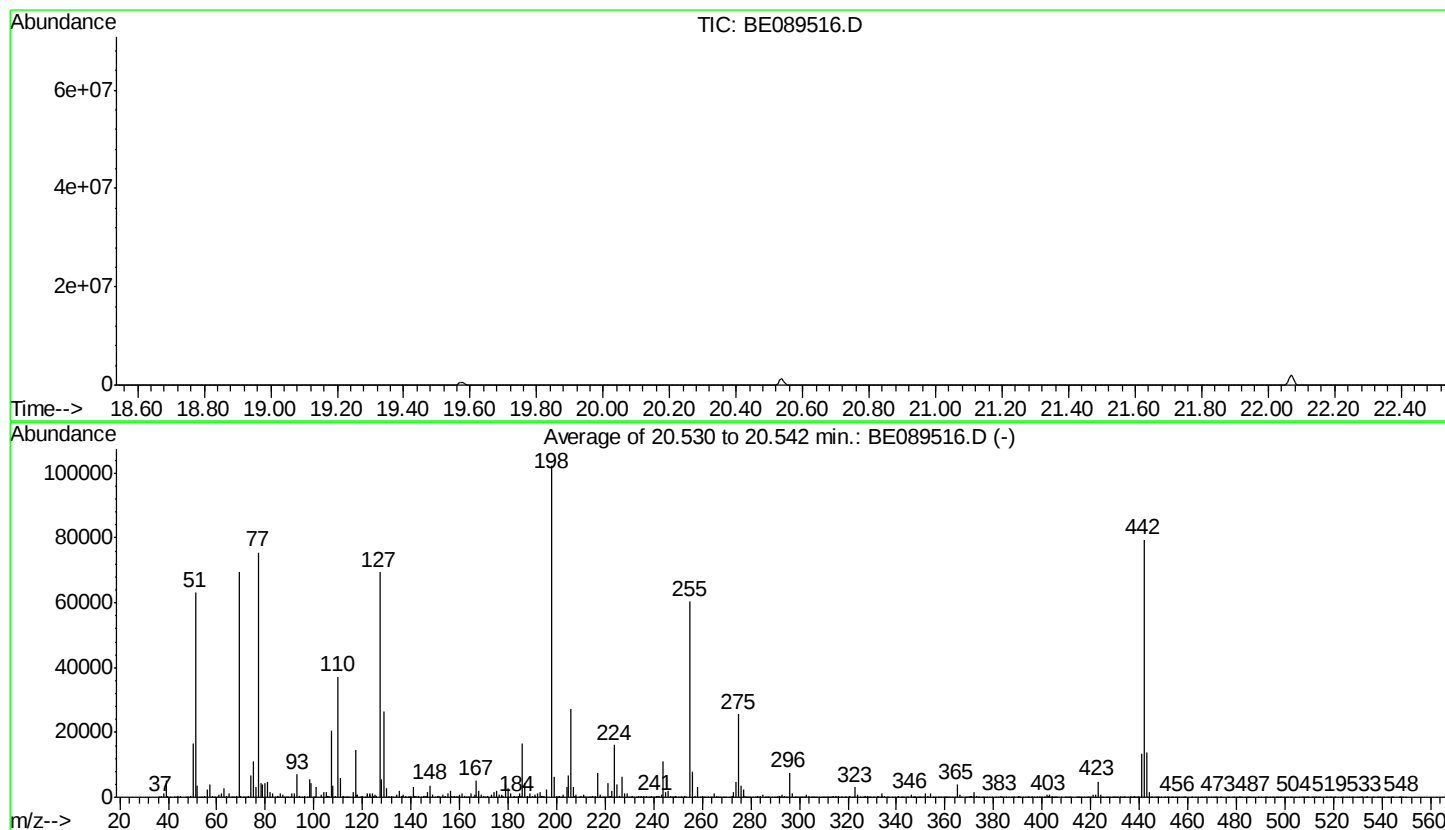

AutoFind: Scans 3258, 3259, 3260; Background Corrected with Scan 3250

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.6	63016	PASS
68	69	0.00	2	0.8	540	PASS
69	198	0.00	100	67.9	69528	PASS
70	69	0.00	2	0.6	424	PASS
127	198	10	80	67.9	69490	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	102325	PASS
199	198	5	9	6.2	6345	PASS
275	198	10	60	24.9	25513	PASS
365	198	1	100	3.8	3849	PASS
441	442	0.01	24	17.1	13602	PASS
442	198	50	100	77.6	79397	PASS
443	442	15	24	17.6	13944	PASS