
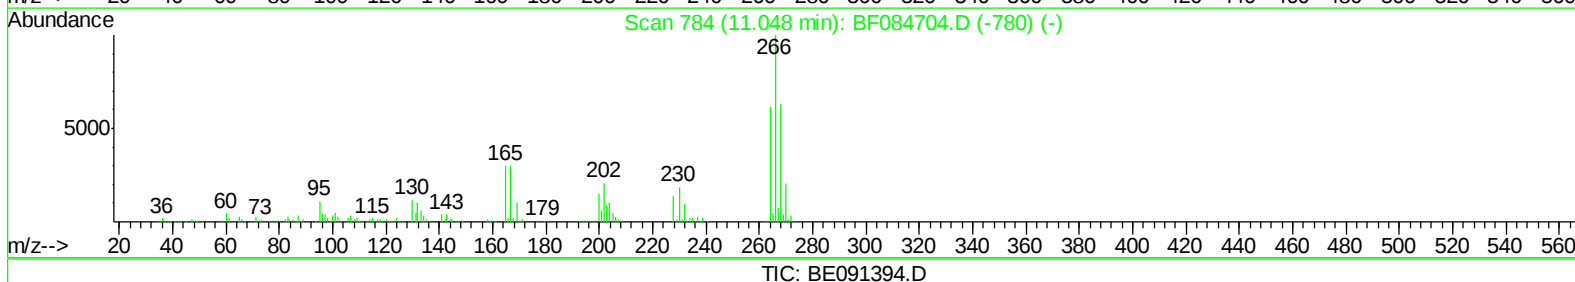
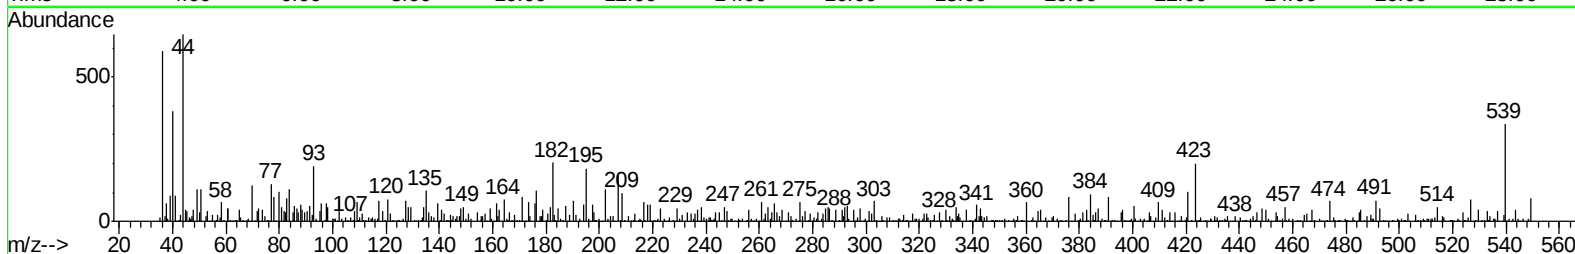


Data Path : Z:\HPCHEM1\BNA E\Data\BE020516\
Data File : BE091394.D
Acq On : 5 Feb 2016 10:40
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 10:34:00 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

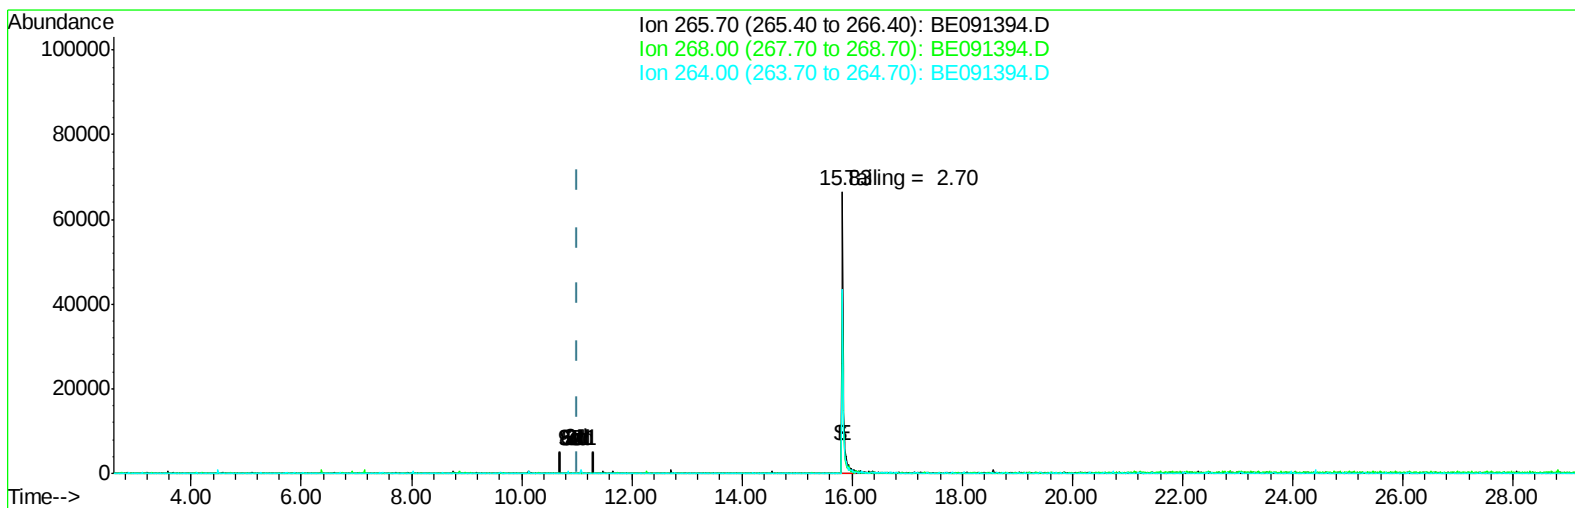

TIC: BE091394.D

(69) Pentachlorophenol (C)




11.280min (+0.266) 81.23ng

response 34

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	67.21
264.00	62.70	62.30
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE020516\
Data File : BE091394.D
Acq On : 5 Feb 2016 10:40
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 10:34:00 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

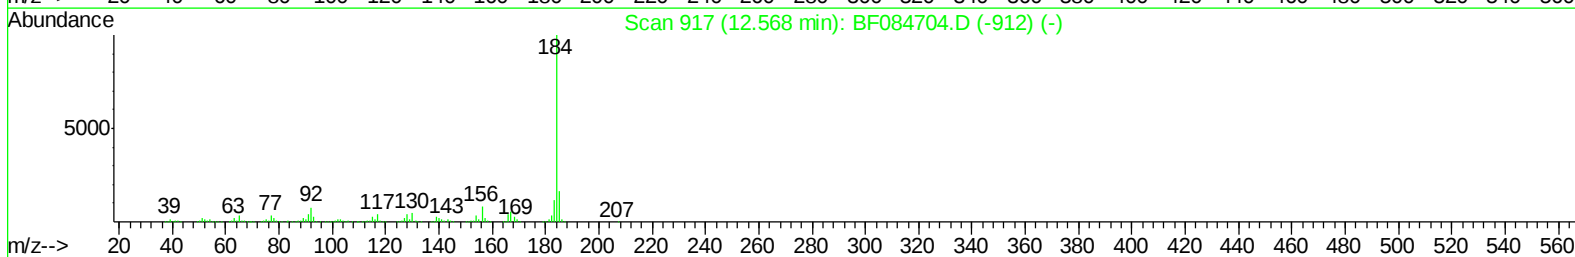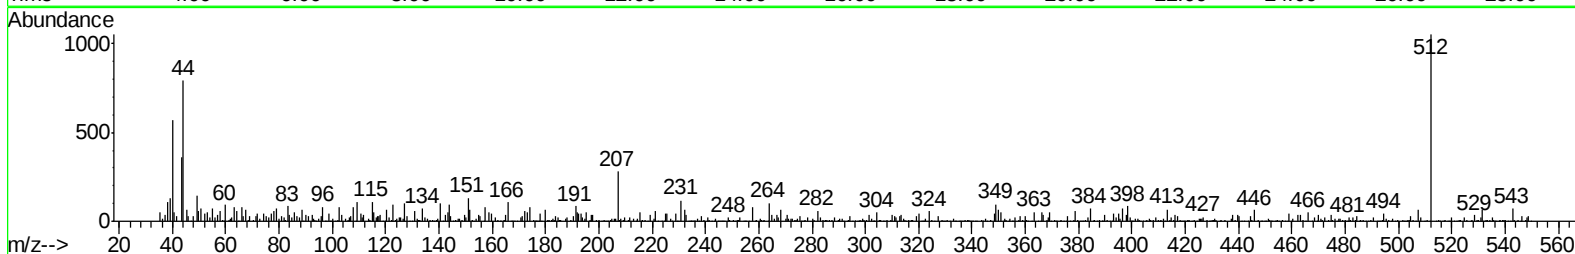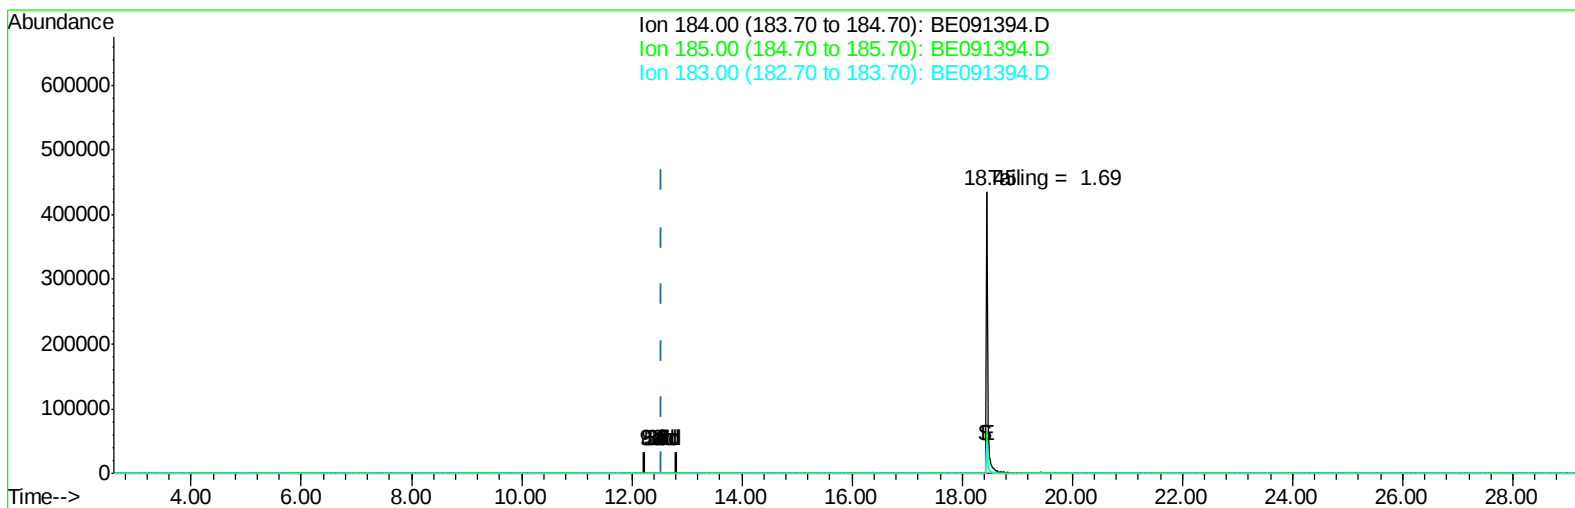

TIC: BE091394.D

(76) Benzidine

12.555min (+0.010) 38.24ng

response 27

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	28.57#
183.00	12.30	65.31#
0.00	0.00	0.00