


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020516\
Data File : BE091394.D
Acq On : 5 Feb 2016 10:40
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 03 00:27:53 2016

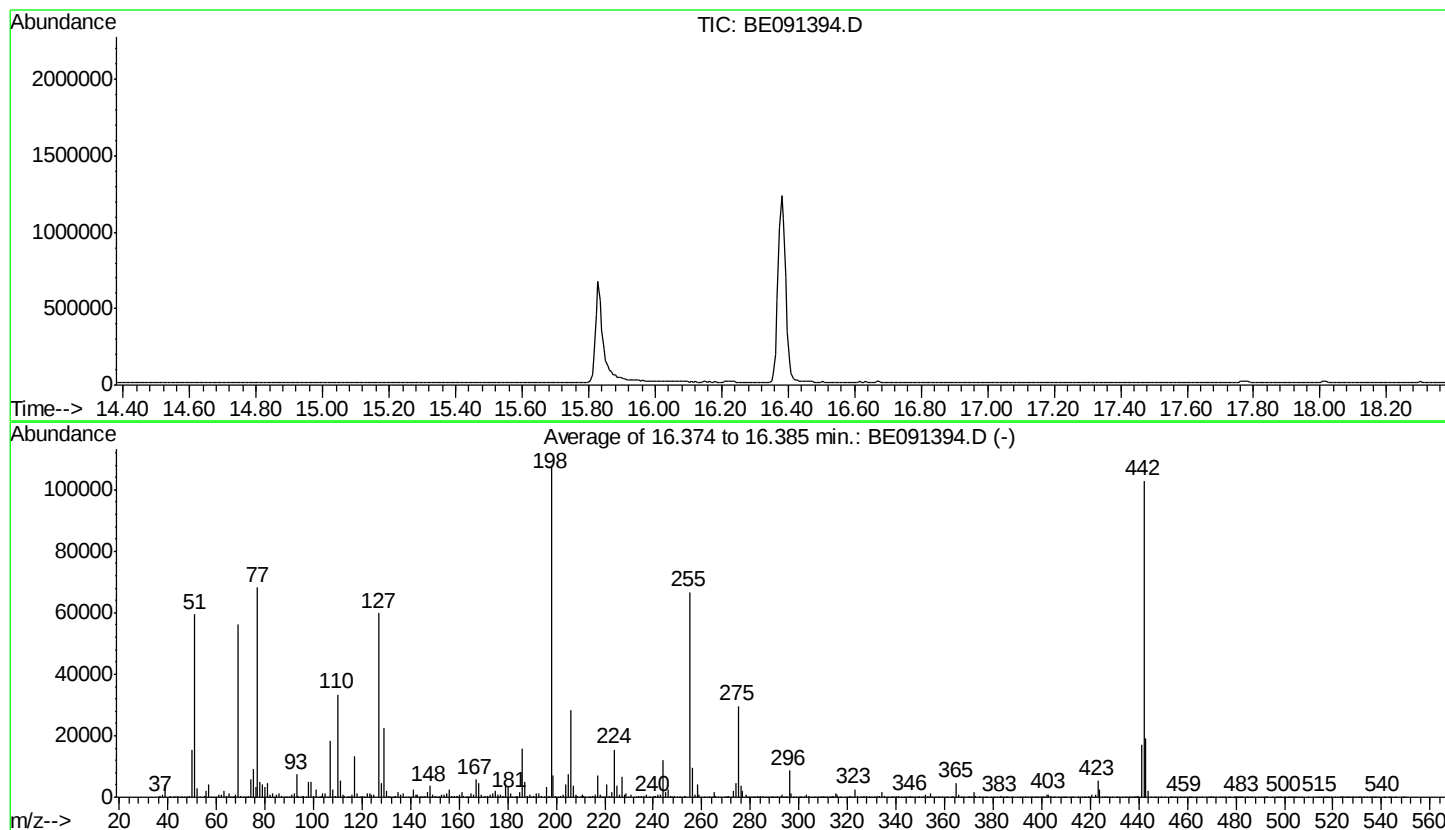

AutoFind: Scans 2346, 2347, 2348; Background Corrected with Scan 2337

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.2	59473	PASS
68	69	0.00	2	1.8	1010	PASS
69	198	0.00	100	52.2	56324	PASS
70	69	0.00	2	0.5	258	PASS
127	198	10	80	55.4	59761	PASS
197	198	0.00	2	0.4	399	PASS
198	198	100	100	100.0	107826	PASS
199	198	5	9	6.7	7221	PASS
275	198	10	60	27.5	29656	PASS
365	198	1	100	4.4	4755	PASS
441	442	0.01	24	16.6	17130	PASS
442	198	50	100	95.4	102888	PASS
443	442	15	24	18.7	19288	PASS