

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095485.D
 Acq On : 5 Feb 2018 11:40
 Operator : SJ/JU
 Sample : J1315-13
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 06 01:31:37 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 01:31:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1649	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4408	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	2810	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7032	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6978	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	8534	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2042	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6228	0.23	ng/ul	0.00
Target Compounds						
17) Pyrene	20.04	202	931	0.040	ng/ul#	1
23) Benzo(a)pyrene	24.26	252	1808	0.067	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095485.D
Acq On : 5 Feb 2018 11:40
Operator : SJ/JU
Sample : J1315-13
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 06 01:31:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 01:31:24 2018
Response via : Initial Calibration




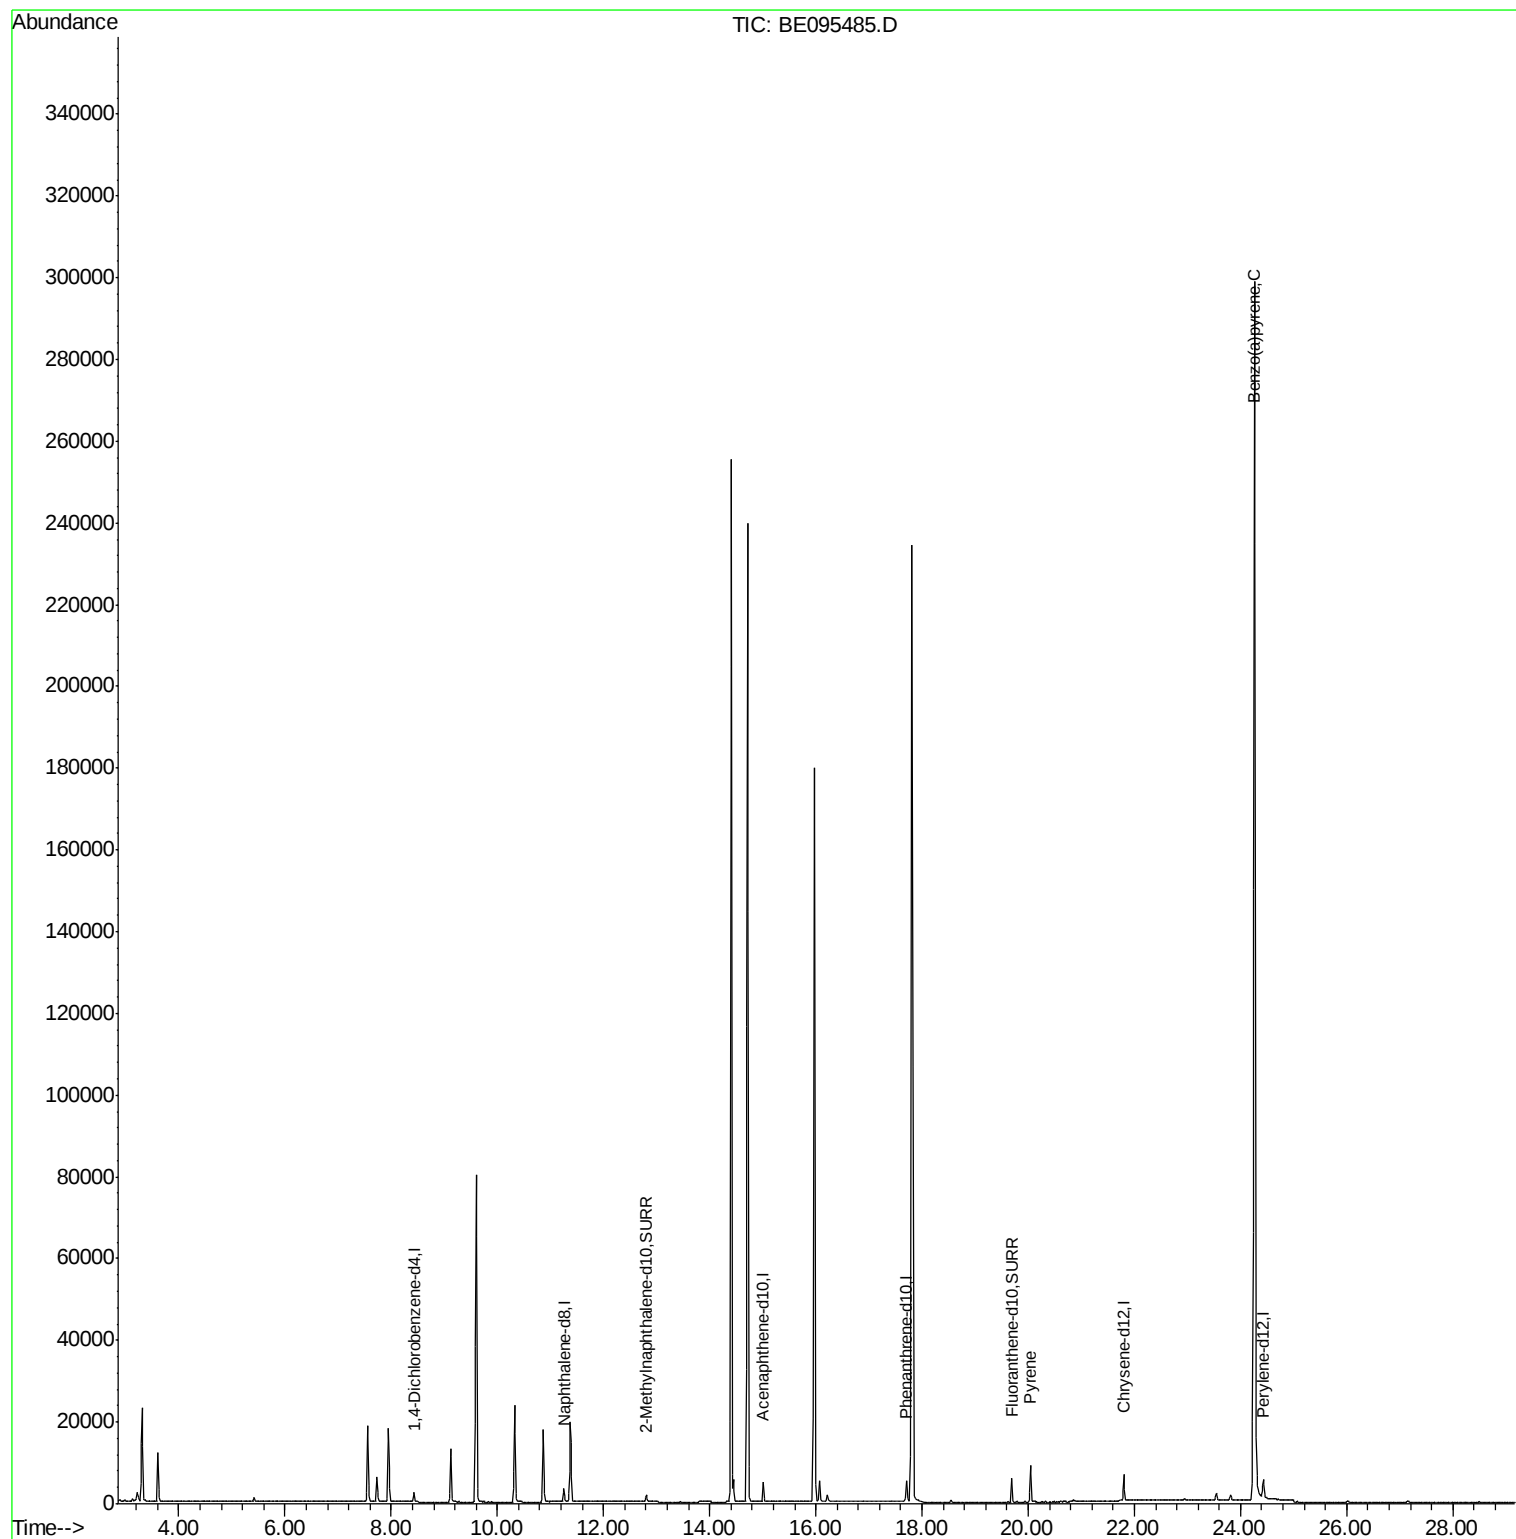


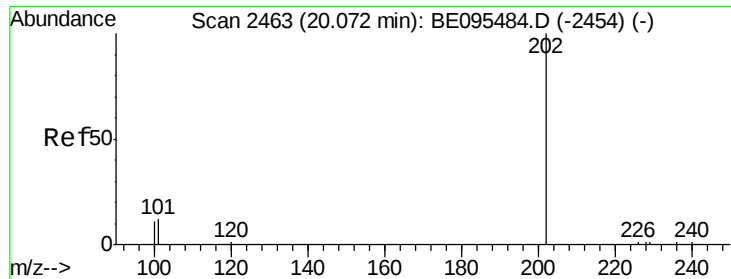

#17
 Pvrene
 Concen: 0.040 ng/ul
 RT: 20.04 min Scan# 2459
 Delta R.T. -0.03 min
 Lab File: BE095485.D
 Acq: 5 Feb 2018 11:40

Instrument :
 BNA_E
 ClientSampled :

Tot Ion:202 Resp: 931
 Ion Ratio Lower Upper
 202 100
 101 176.6 18.2 27.4#
 100 1201.3 15.6 23.4#

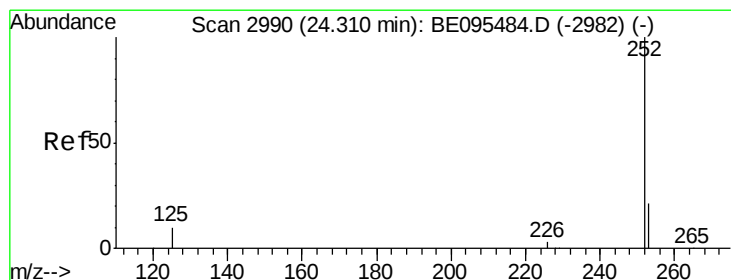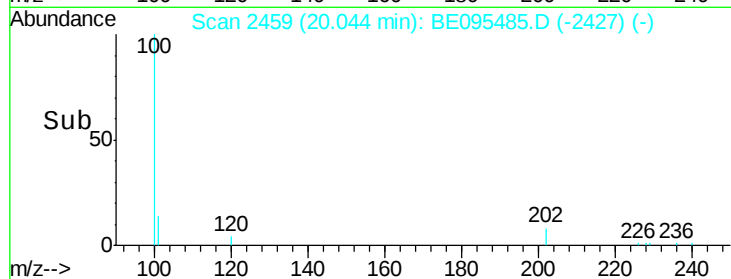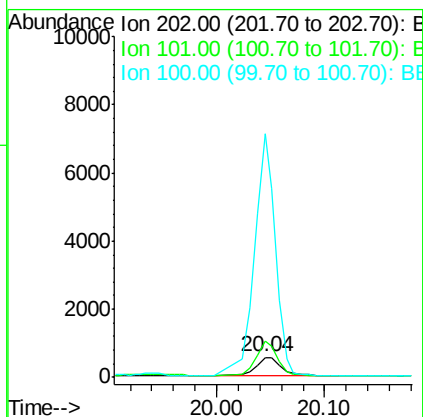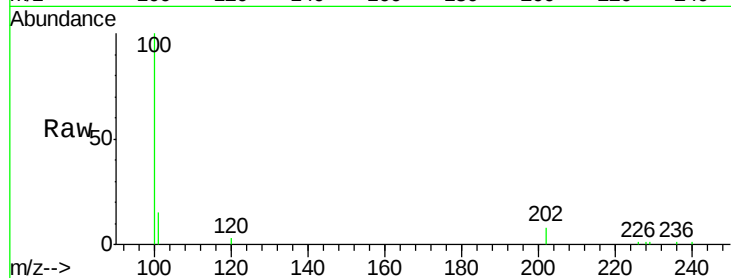

#23
 Benzo(a)pyrene
 Concen: 0.067 ng/ul
 RT: 24.26 min Scan# 2985
 Delta R.T. -0.05 min
 Lab File: BE095485.D
 Acq: 5 Feb 2018 11:40

Tgt Ion:252 Resp: 1808
 Ion Ratio Lower Upper
 252 100
 253 47.4 28.5 42.7#
 125 72.9 18.1 27.1#

