

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095486.D
 Acq On : 5 Feb 2018 12:24
 Operator : SJ/JU
 Sample : J1315-11
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 06 01:31:43 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 01:31:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1677	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4559	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	2861	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6542	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6695	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	407359	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2469	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6966	0.28	ng/ul	0.00
Target Compounds						
17) Pyrene	20.04	202	1109	0.049	ng/ul#	Ovalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095486.D
Acq On : 5 Feb 2018 12:24
Operator : SJ/JU
Sample : J1315-11
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 06 01:31:43 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 01:31:24 2018
Response via : Initial Calibration

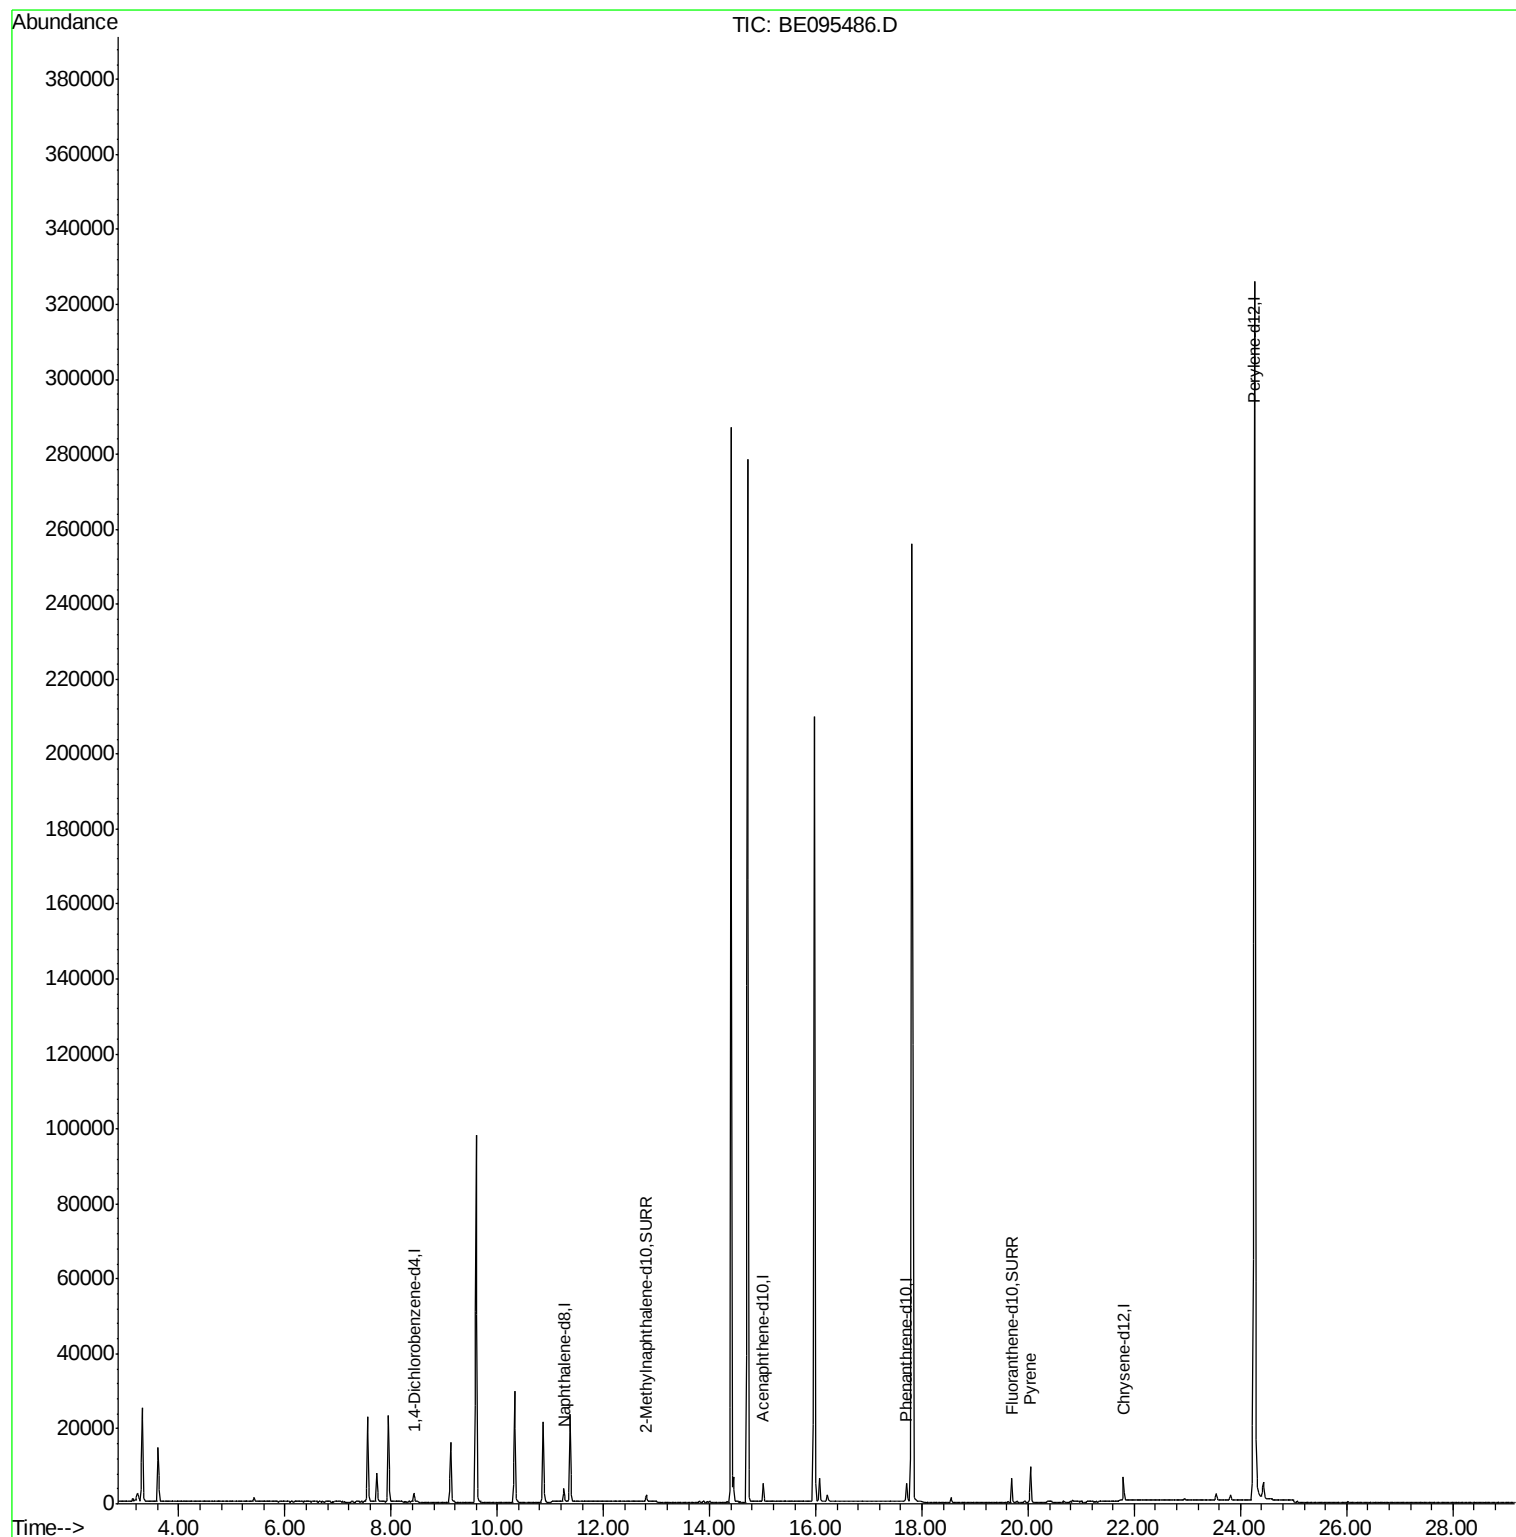

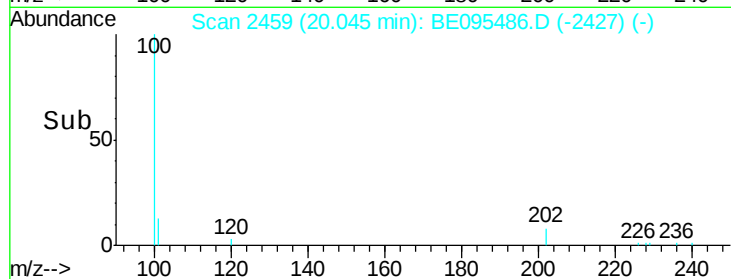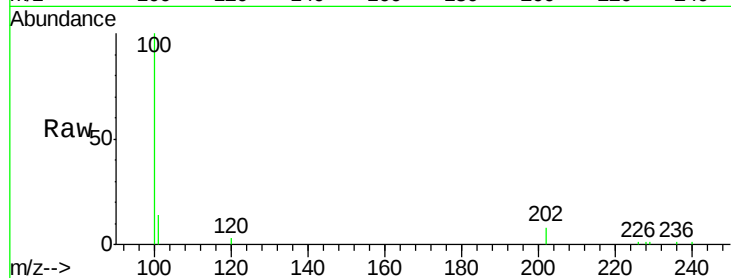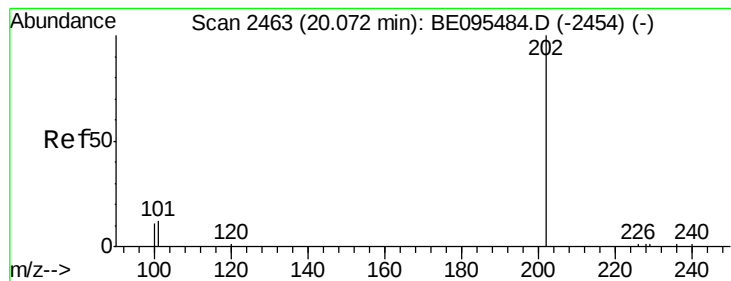

#17

Pvrene

Concen: 0.049 ng/ul

RT: 20.04 min Scan# 2459

Delta R.T. -0.03 min

Lab File: BE095486.D

Acq: 5 Feb 2018 12:24

Instrument :

BNA_E

ClientSampleId :

Tot Ion:202 Resp: 1109

Ion Ratio Lower Upper

202 100

101 169.8 18.2 27.4#

100 1184.7 15.6 23.4#

