

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095487.D
 Acq On : 5 Feb 2018 13:00
 Operator : SJ/JU
 Sample : J1315-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 06 01:31:48 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 01:31:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1614	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4453	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	2798	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6433	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6830	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	8164	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2134	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6213	0.25	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	44	0.035	ng/ul#	71
17) Pyrene	20.05	202	1025	0.045	ng/ul#	1
23) Benzo(a)pyrene	24.26	252	1729	0.067	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095487.D
Acq On : 5 Feb 2018 13:00
Operator : SJ/JU
Sample : J1315-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 06 01:31:48 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 01:31:24 2018
Response via : Initial Calibration




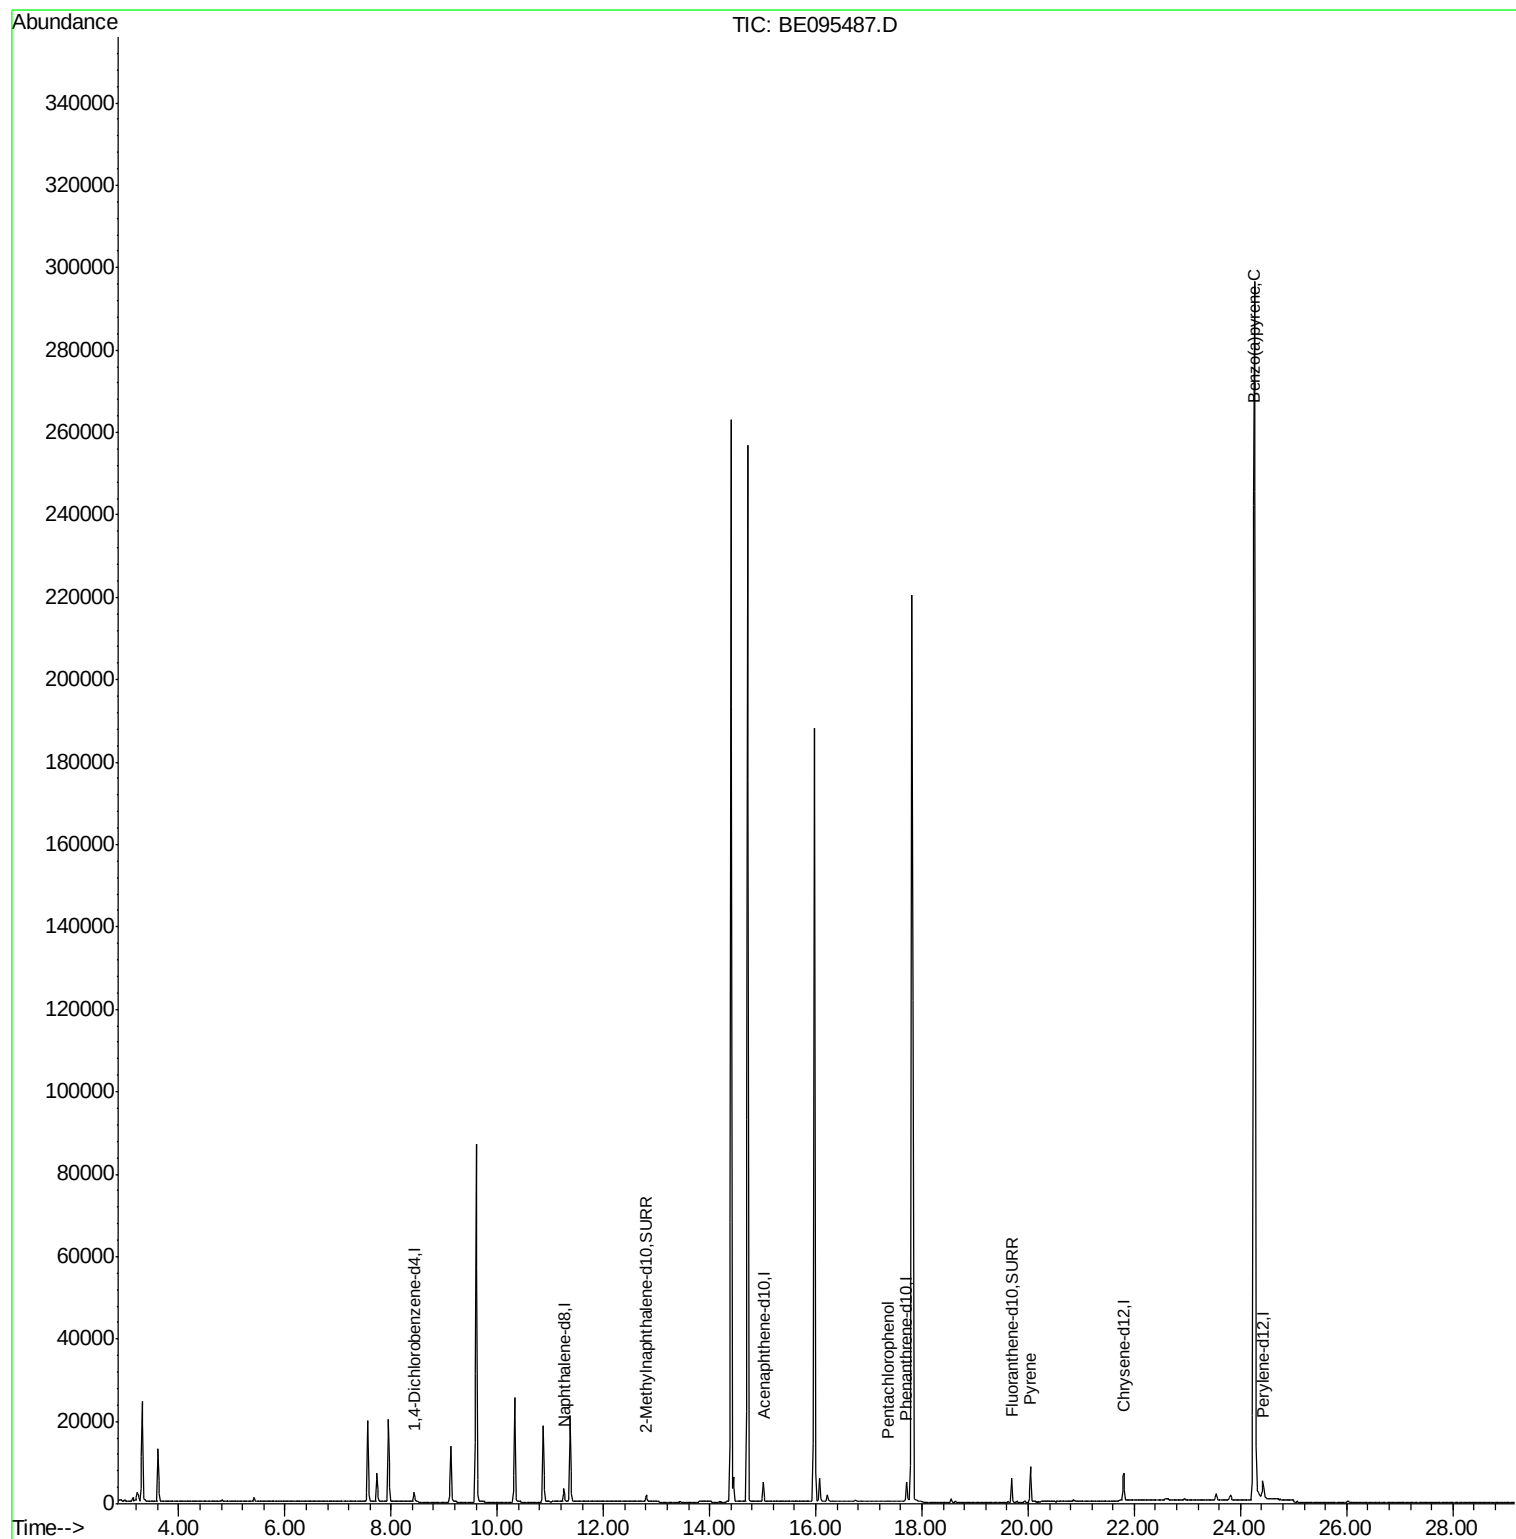


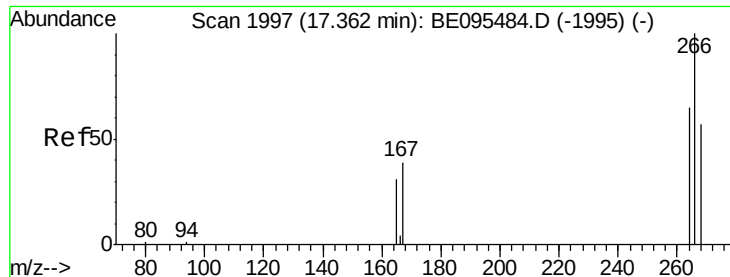

#11
 Pentachlorophenol
 Concen: 0.035 ng/ul
 RT: 17.36 min Scan# 1998
 Delta R.T. -0.00 min
 Lab File: BE095487.D
 Acq: 5 Feb 2018 13:00




Instrument :
 BNA_E
 ClientSampleId :




Tot Ion:266 Resp: 44
 Ion Ratio Lower Upper
 266 100
 264 72.7 47.9 71.9#
 268 93.2 49.8 74.8#

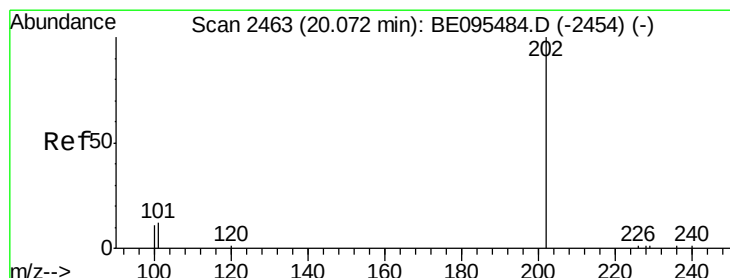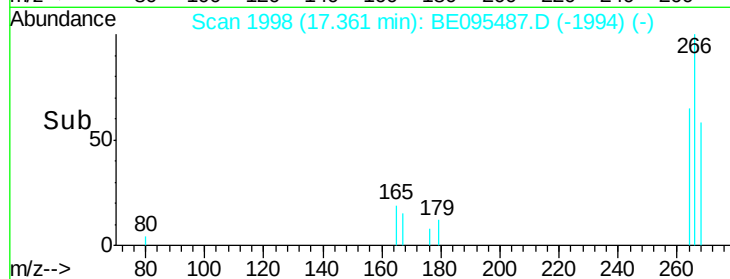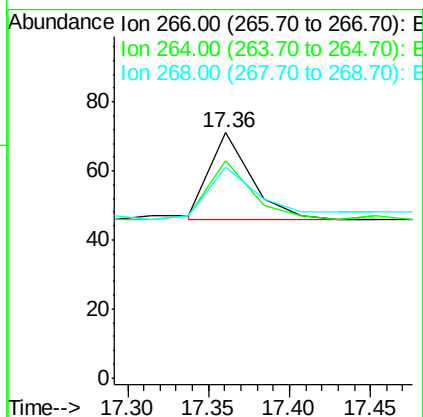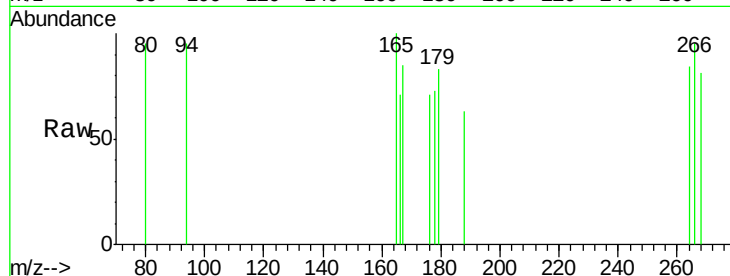

#17
 Pyrene
 Concen: 0.045 ng/ul
 RT: 20.05 min Scan# 2461
 Delta R.T. -0.03 min
 Lab File: BE095487.D
 Acq: 5 Feb 2018 13:00

Tgt Ion:202 Resp: 1025
 Ion Ratio Lower Upper
 202 100
 101 173.5 18.2 27.4#
 100 1159.6 15.6 23.4#

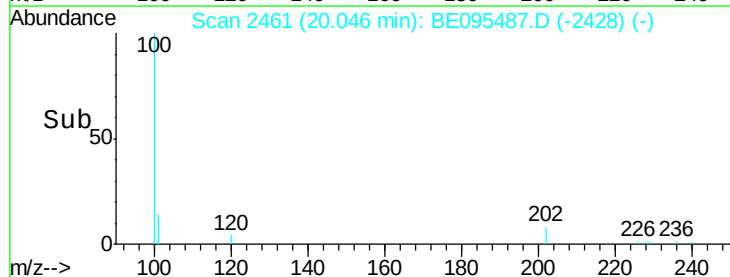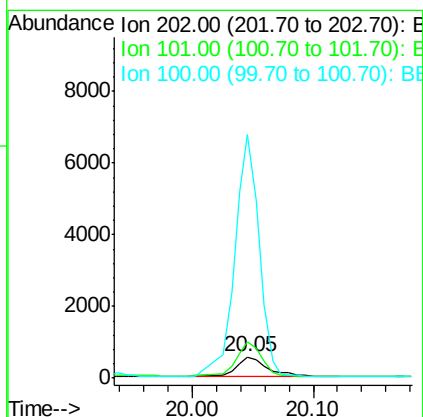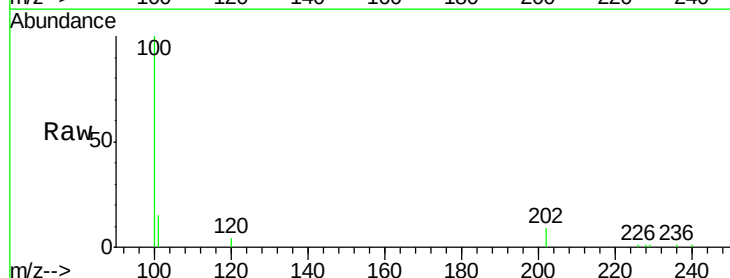

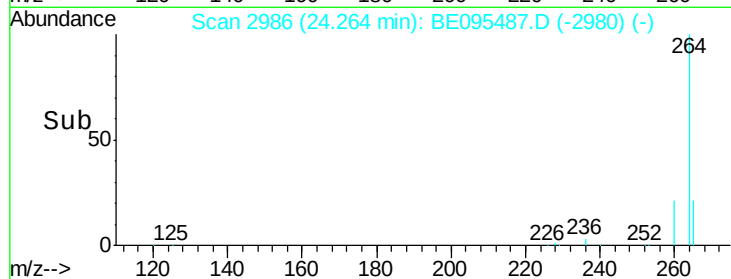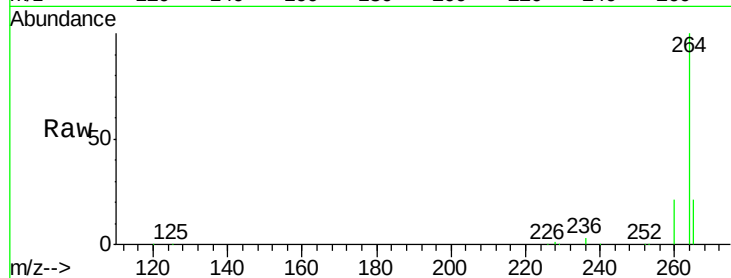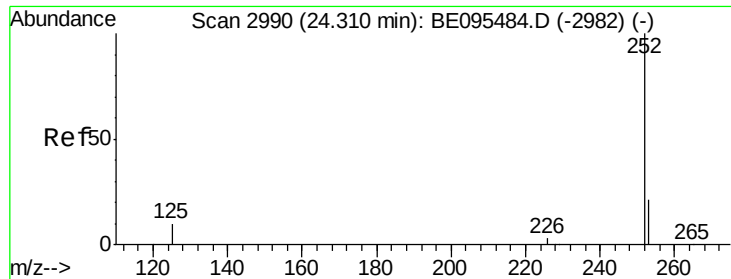

#23

Benzo(a)pyrene

Concen: 0.067 ng/ul

RT: 24.26 min Scan# 2986

Delta R.T. -0.05 min

Lab File: BE095487.D

Acq: 5 Feb 2018 13:00

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 252 Resp: 1729

Ion Ratio Lower Upper

252 100

253 44.2 28.5 42.7#

125 56.9 18.1 27.1#

