

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095488.D
 Acq On : 5 Feb 2018 13:36
 Operator : SJ/JU
 Sample : J1315-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 06 01:31:55 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 01:31:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1717	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4795	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3003	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6944	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7214	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	8566	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2196	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6250	0.24	ng/ul	0.00
Target Compounds						
17) Pyrene	20.05	202	964	0.040	ng/ul#	1
23) Benzo(a)pyrene	24.27	252	1794	0.066	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095488.D
Acq On : 5 Feb 2018 13:36
Operator : SJ/JU
Sample : J1315-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 06 01:31:55 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 01:31:24 2018
Response via : Initial Calibration




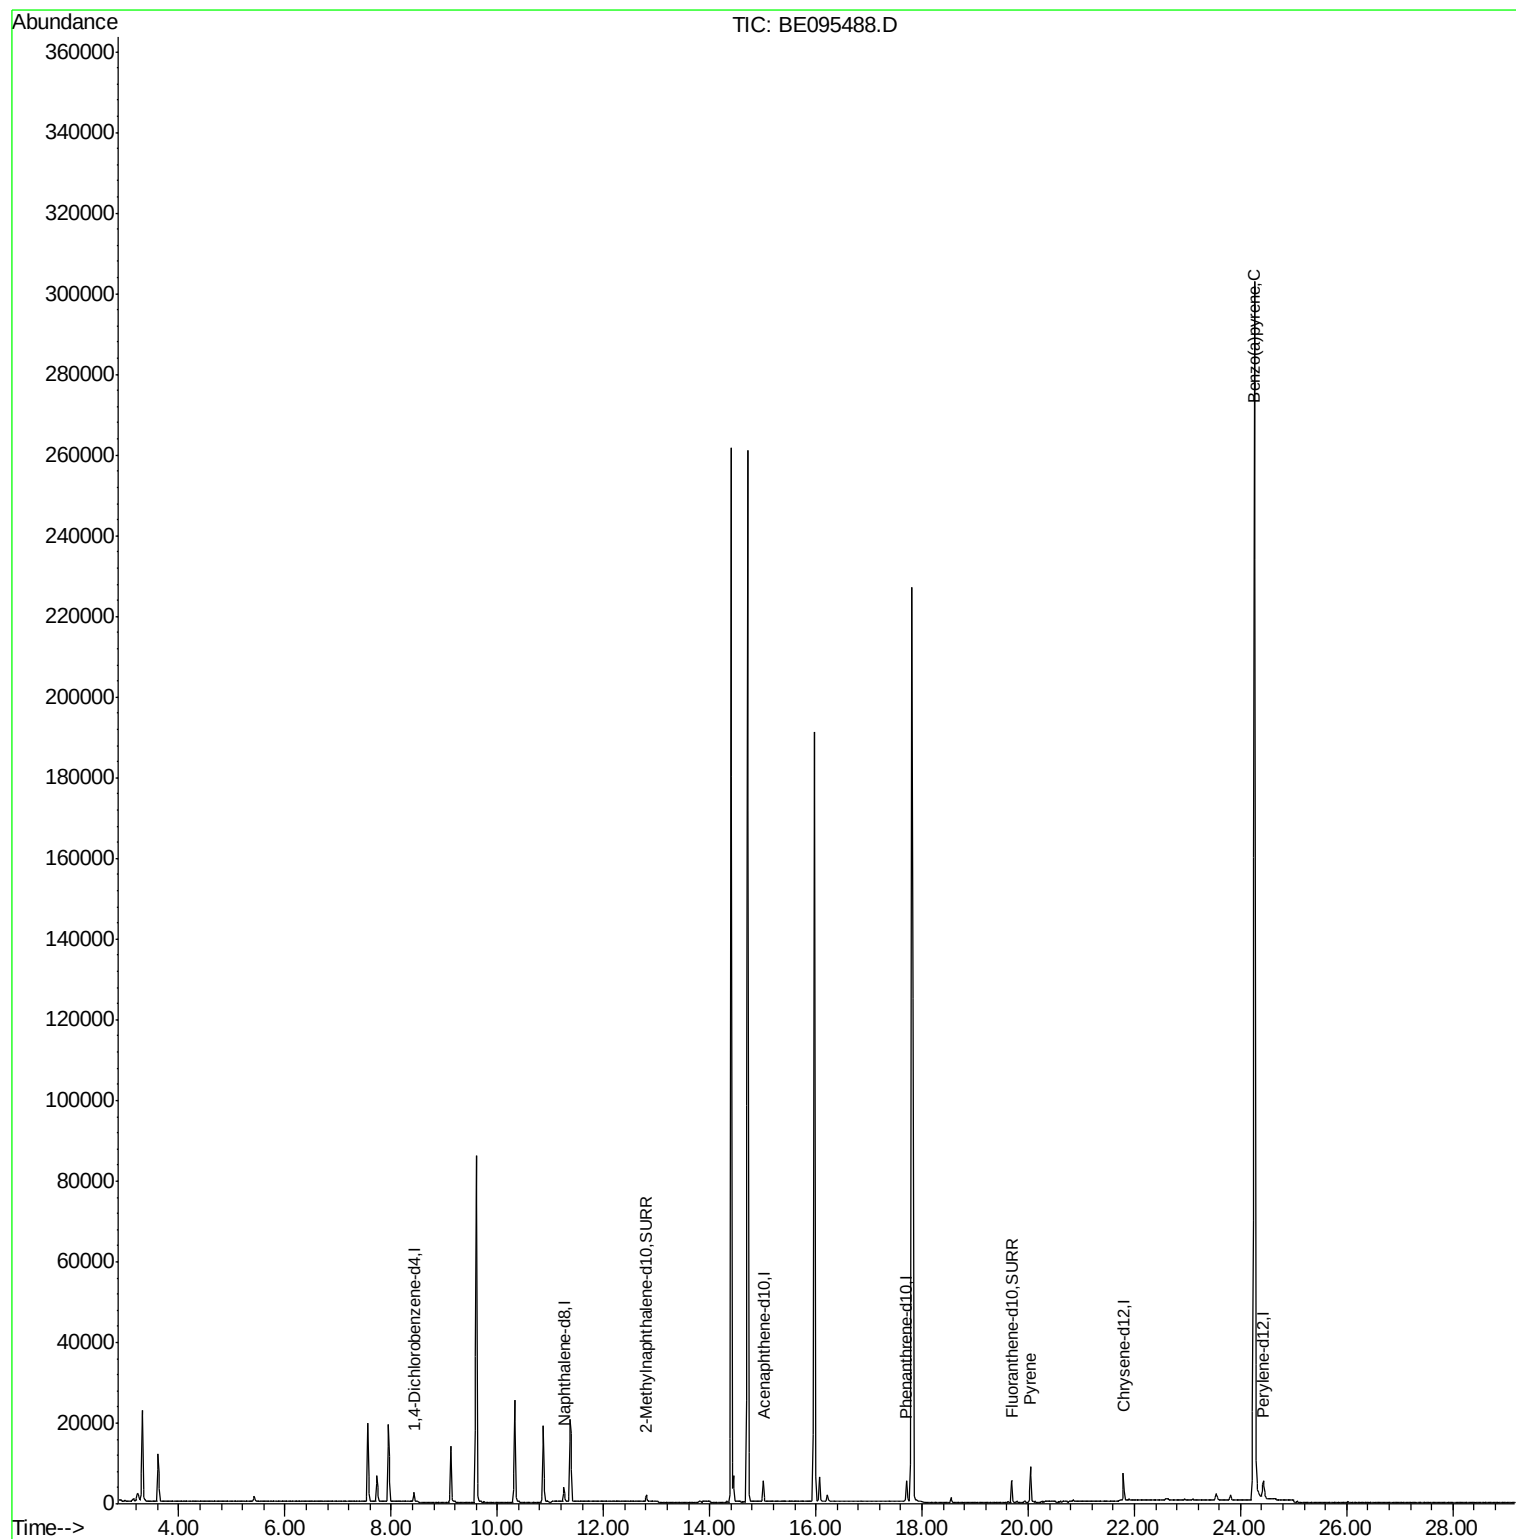


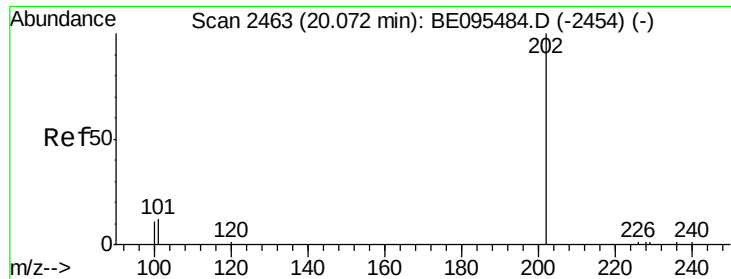

#17
Pvrene
Concen: 0.040 ng/ul
RT: 20.05 min Scan# 2459
Delta R.T. -0.03 min
Lab File: BE095488.D
Acq: 5 Feb 2018 13:36

Instrument :
BNA_E
ClientSampleId :

Tot Ion:202 Resp: 964
Ion Ratio Lower Upper
202 100
101 173.8 18.2 27.4#
100 1204.6 15.6 23.4#

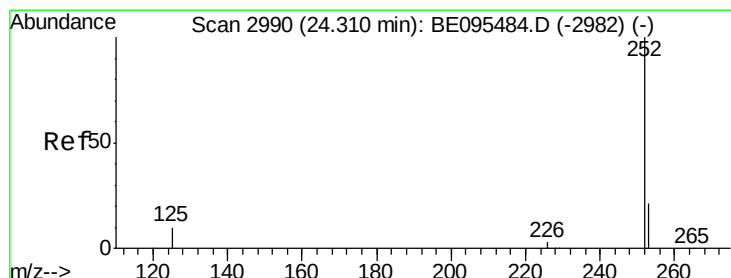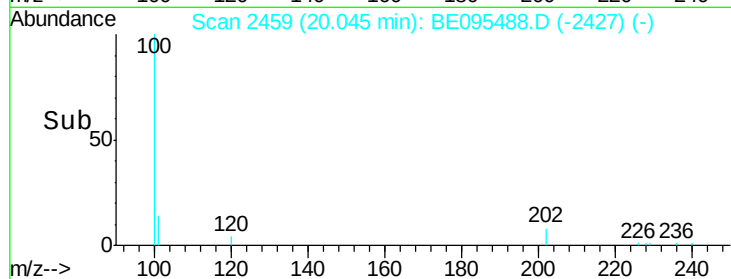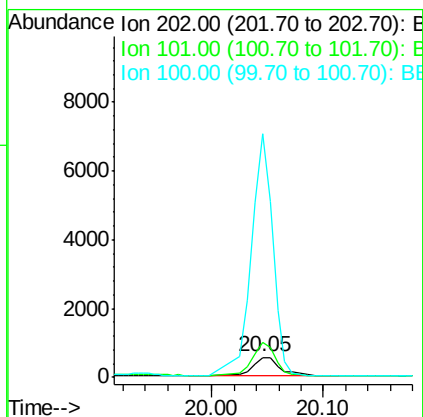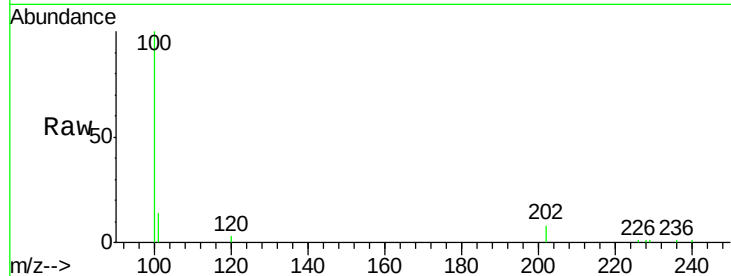

#23
Benzo(a)pyrene
Concen: 0.066 ng/ul
RT: 24.27 min Scan# 2985
Delta R.T. -0.04 min
Lab File: BE095488.D
Acq: 5 Feb 2018 13:36

Tgt Ion:252 Resp: 1794
Ion Ratio Lower Upper
252 100
253 46.7 28.5 42.7#
125 52.4 18.1 27.1#

