

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095490.D
 Acq On : 5 Feb 2018 14:48
 Operator : SJ/JU
 Sample : J1315-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 06 01:32:07 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 01:31:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1716	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	4739	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	2978	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6797	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6747	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	8084	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2591	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7302	0.28	ng/ul	0.00
Target Compounds						
17) Pyrene	20.05	202	1133	0.050	ng/ul#	1
23) Benzo(a)pyrene	24.27	252	1947	0.076	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095490.D
Acq On : 5 Feb 2018 14:48
Operator : SJ/JU
Sample : J1315-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 06 01:32:07 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 01:31:24 2018
Response via : Initial Calibration

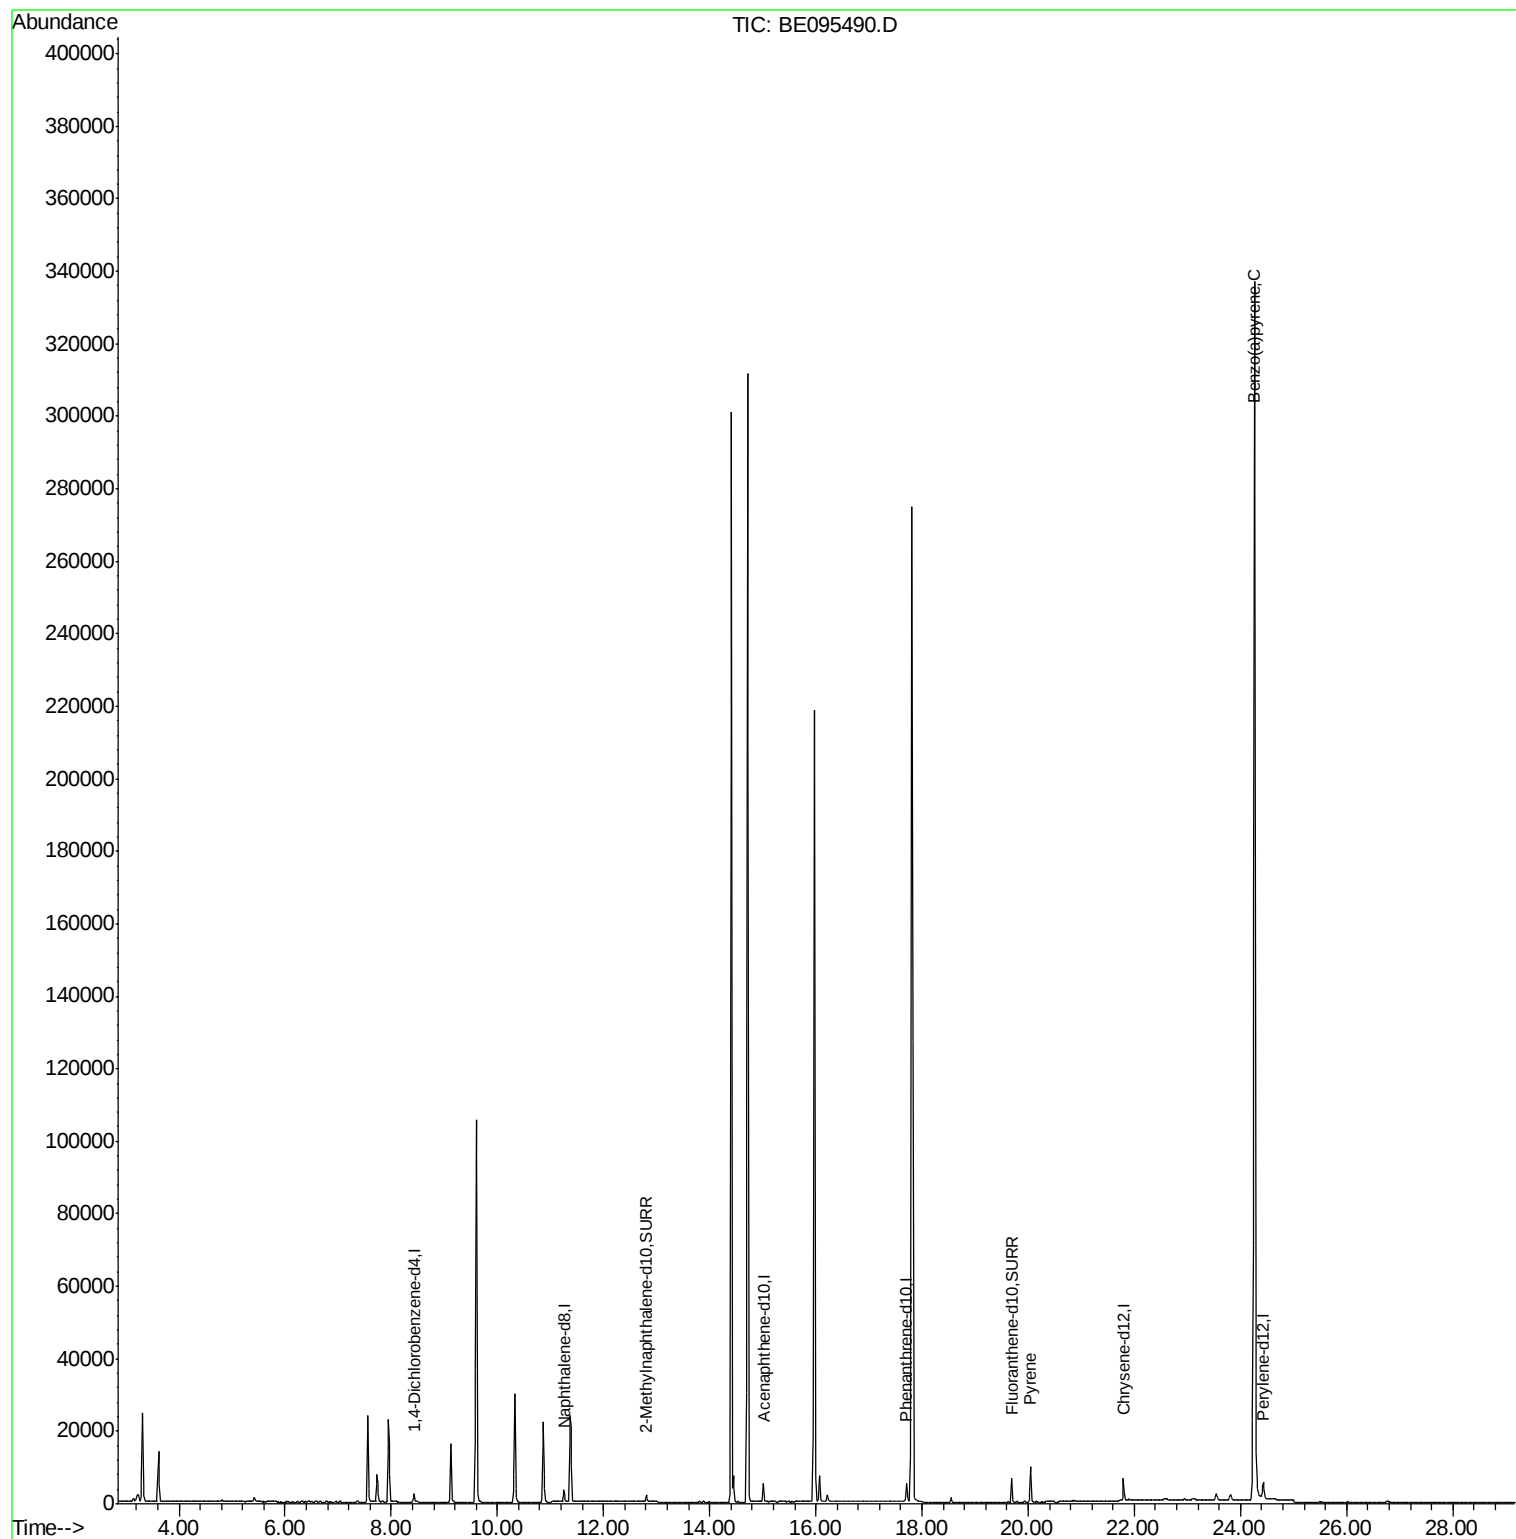


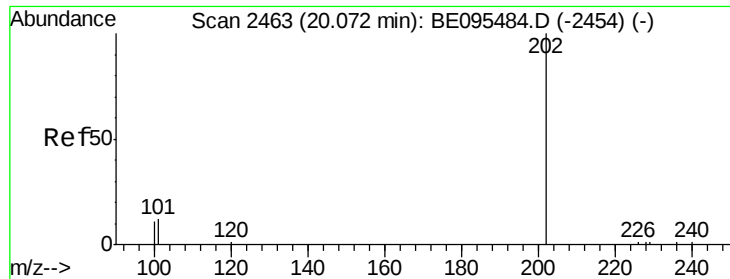




#17
Pvrene
Concen: 0.050 ng/ul
RT: 20.05 min Scan# 2460
Delta R.T. -0.02 min
Lab File: BE095490.D
Acq: 5 Feb 2018 14:48

Instrument :
BNA_E
ClientSampleId :

Tot Ion:202 Resp: 1133
Ion Ratio Lower Upper
202 100
101 155.6 18.2 27.4#
100 943.7 15.6 23.4#

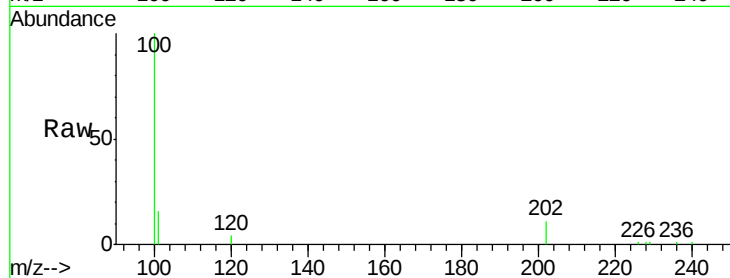


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

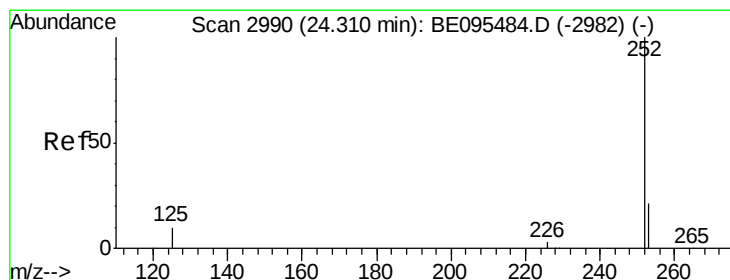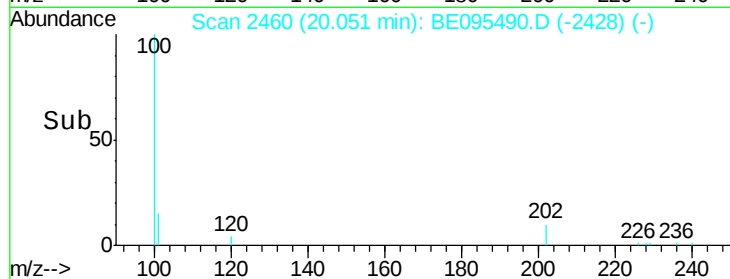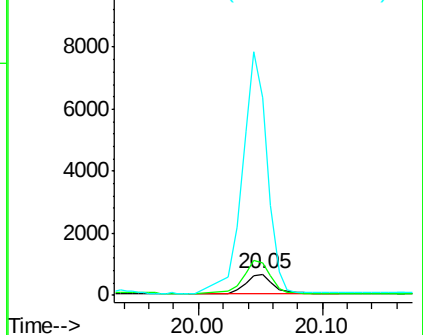

#23
Benzo(a)pyrene
Concen: 0.076 ng/ul
RT: 24.27 min Scan# 2985
Delta R.T. -0.04 min
Lab File: BE095490.D
Acq: 5 Feb 2018 14:48

Tgt Ion:252 Resp: 1947
Ion Ratio Lower Upper
252 100
253 43.1 28.5 42.7#
125 55.4 18.1 27.1#

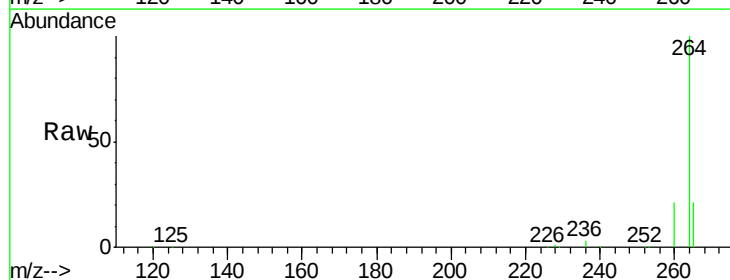

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

