

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095499.D
 Acq On : 5 Feb 2018 20:10
 Operator : SJ/JU
 Sample : J1296-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 06 02:10:37 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 02:09:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1814	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5067	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3174	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7309	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7444	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	348382	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2792	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7859	0.28	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.30	128	2988	0.211	ng/ul#	90
11) Pentachlorophenol	17.36	266	9305	6.573	ng/ul	97
12) Phenanthrene	17.75	178	618	0.025	ng/ul#	65
17) Pyrene	20.05	202	1361	0.054	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095499.D
Acq On : 5 Feb 2018 20:10
Operator : SJ/JU
Sample : J1296-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 06 02:10:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration

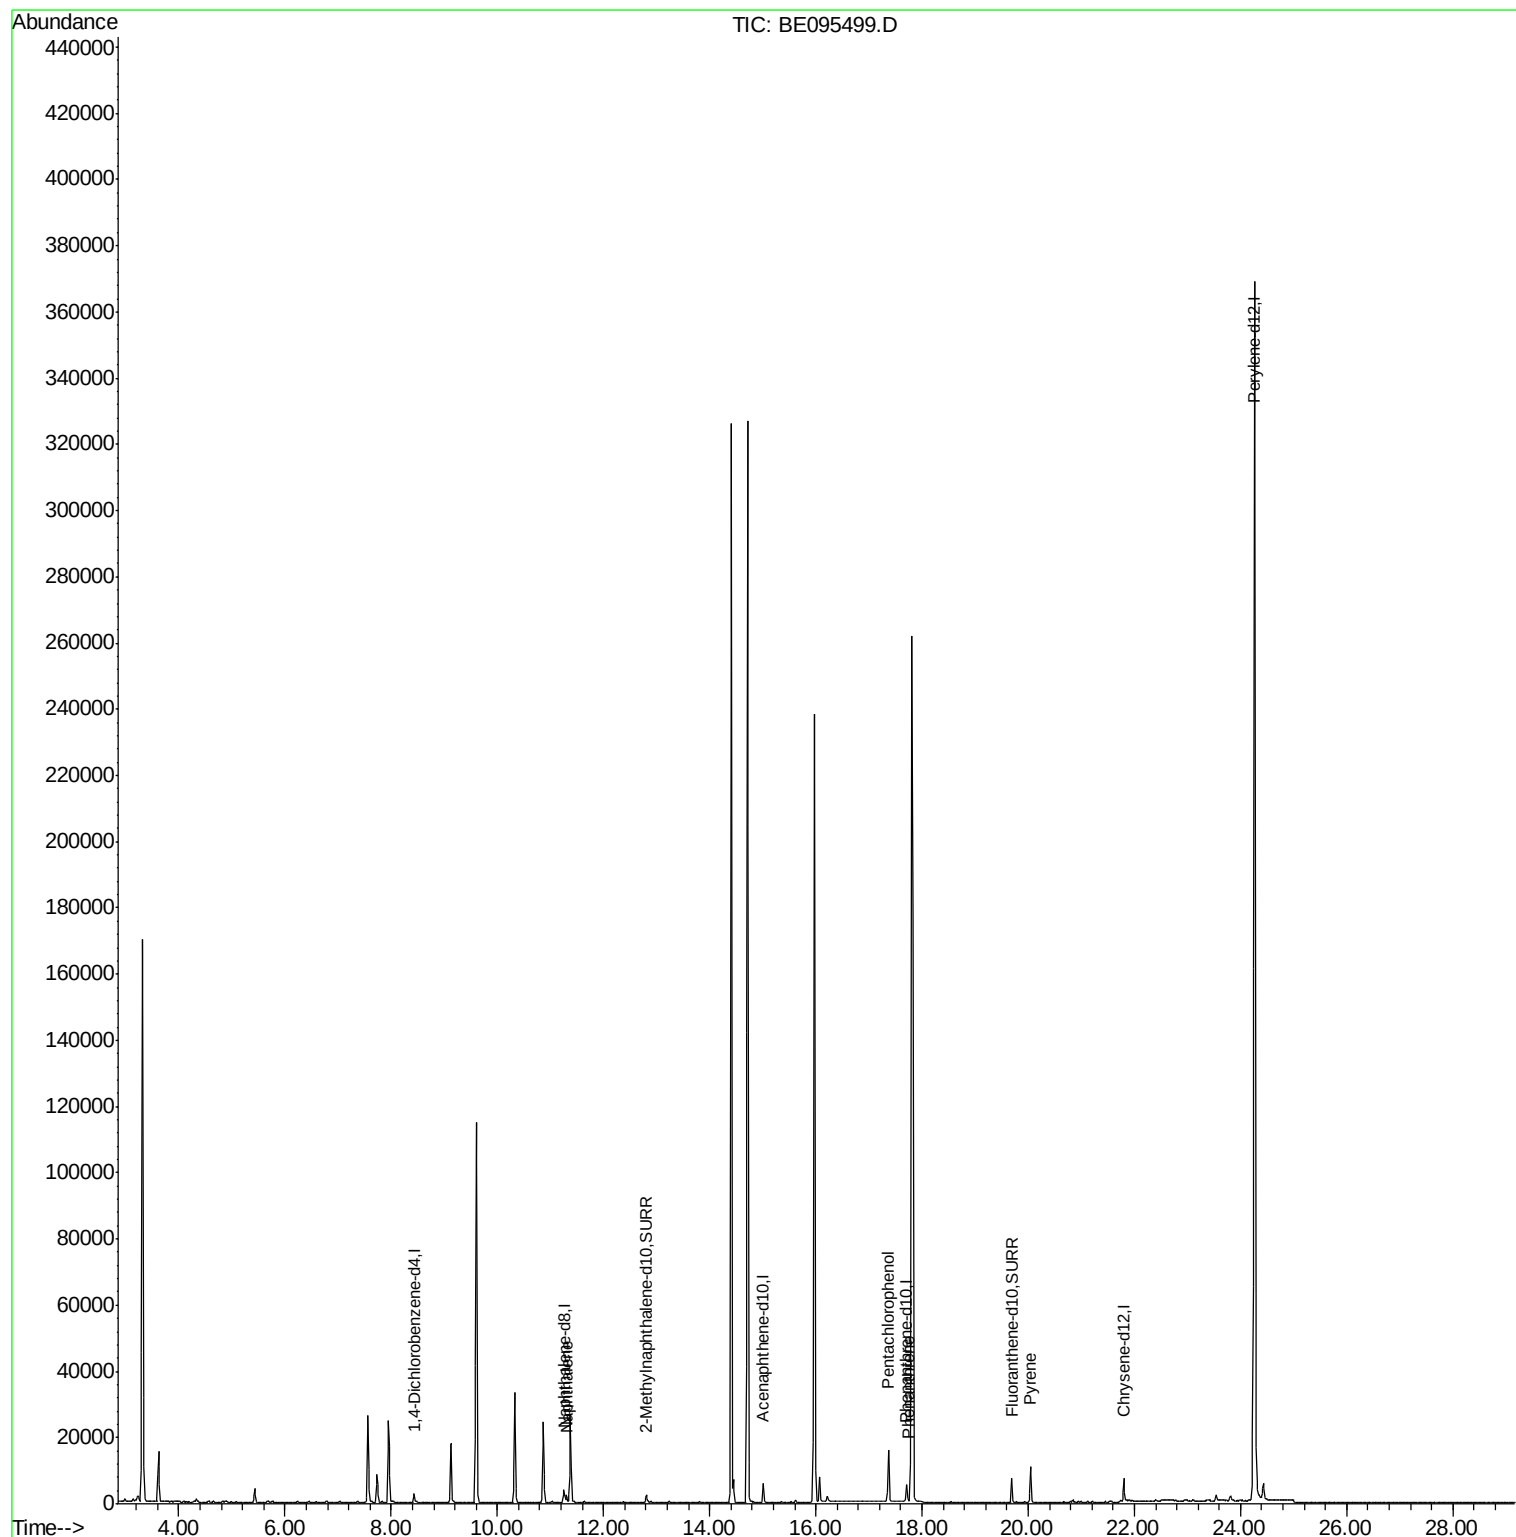

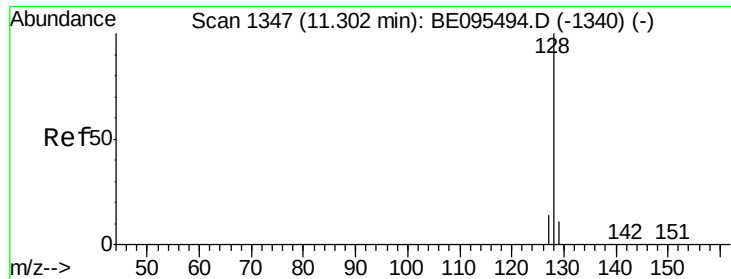

#3

Naphthalene

Concen: 0.211 ng/ul

RT: 11.30 min Scan# 1347

Delta R.T. 0.00 min

Lab File: BE095499.D

Acq: 5 Feb 2018 20:10

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 2988

Ion Ratio Lower Upper

128 100

129 13.3 11.3 16.9




127 15.4 4.0 6.0#

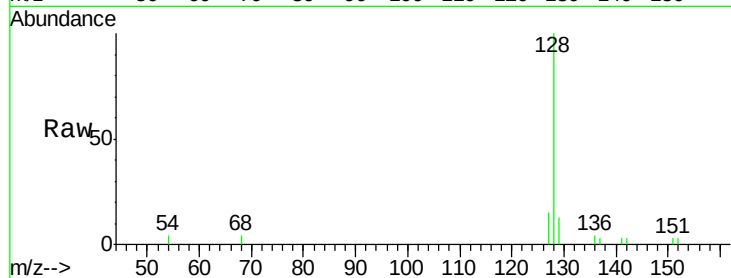

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

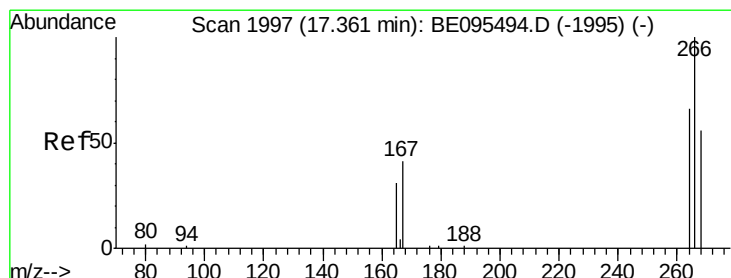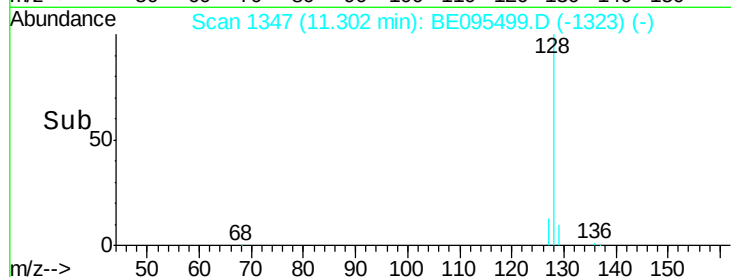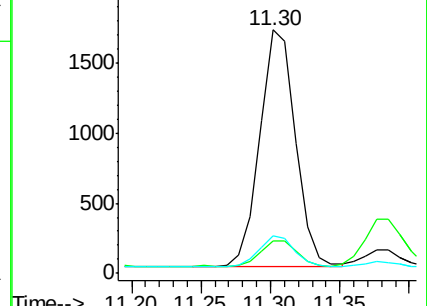

#11

Pentachlorophenol

Concen: 6.573 ng/ul

RT: 17.36 min Scan# 1997

Delta R.T. 0.00 min

Lab File: BE095499.D

Acq: 5 Feb 2018 20:10


Tgt Ion:266 Resp: 9305

Ion Ratio Lower Upper

266 100

264 63.4 47.9 71.9



268 62.8 49.8 74.8

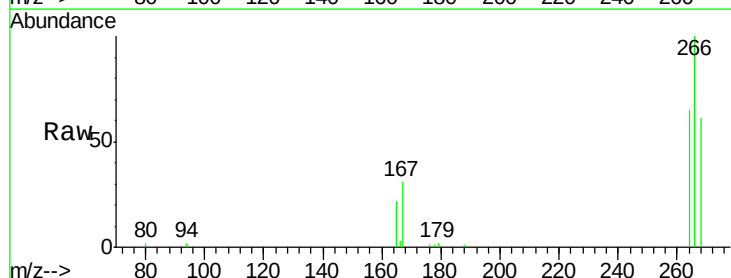


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

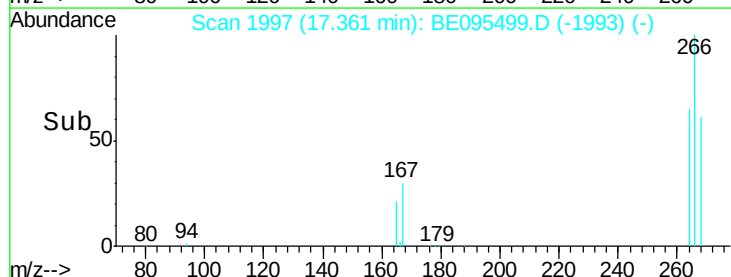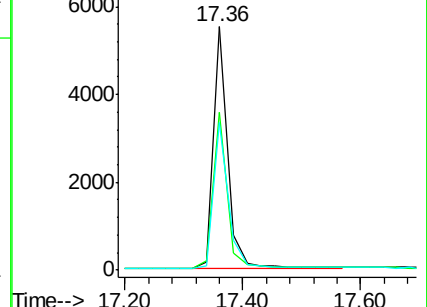

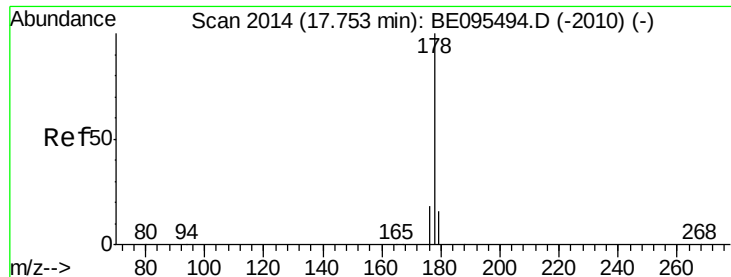

#12

Phenanthrene

Concen: 0.025 ng/ul

RT: 17.75 min Scan# 2014

Delta R.T. 0.00 min

Lab File: BE095499.D

Acq: 5 Feb 2018 20:10

Instrument :

BNA_E

ClientSampleId :


Tot Ion:178 Resp: 618

Ion Ratio Lower Upper

178 100

179 38.5 18.4 27.6#




176 34.4 13.6 20.4#

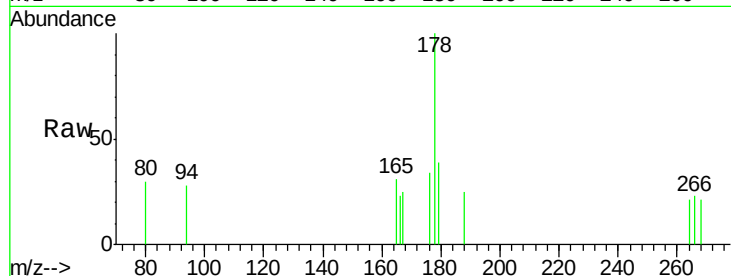

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

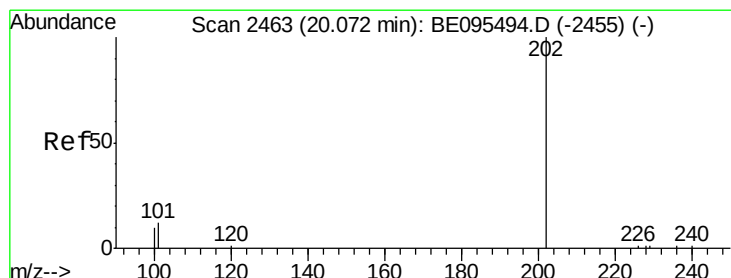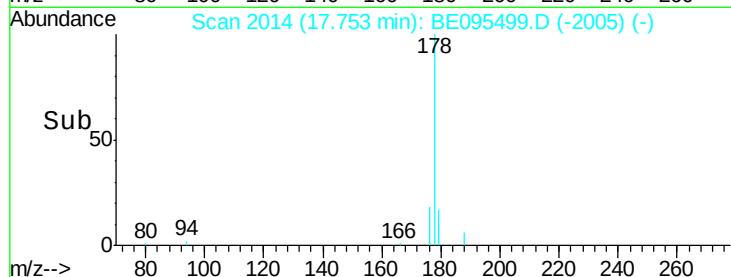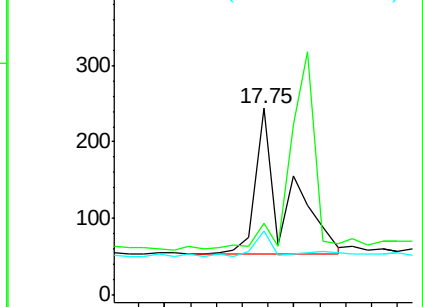

#17

Pyrene

Concen: 0.054 ng/ul

RT: 20.05 min Scan# 2459

Delta R.T. -0.03 min

Lab File: BE095499.D

Acq: 5 Feb 2018 20:10


Tgt Ion:202 Resp: 1361

Ion Ratio Lower Upper

202 100

101 176.4 18.2 27.4#

100 1260.5 15.6 23.4#

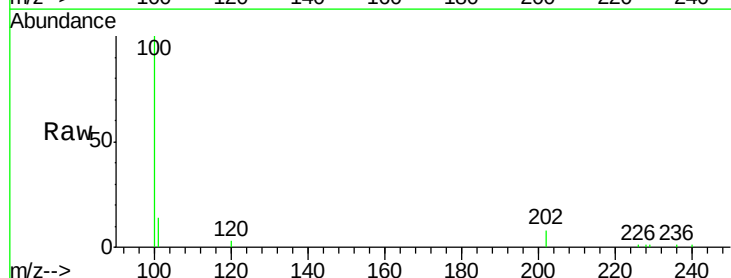

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

