

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095506.D
 Acq On : 6 Feb 2018 00:21
 Operator : SJ/JU
 Sample : J1314-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 06 02:11:31 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 02:09:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1679	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4761	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	2963	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6884	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7588	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	324026	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2275	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6898	0.26	ng/ul	0.00
Target Compounds						
					Ovalue	
11) Pentachlorophenol	17.36	266	39	0.029	ng/ul#	86
12) Phenanthrene	17.75	178	503	0.022	ng/ul#	47
17) Pyrene	20.05	202	1083	0.043	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095506.D
Acq On : 6 Feb 2018 00:21
Operator : SJ/JU
Sample : J1314-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 06 02:11:31 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration




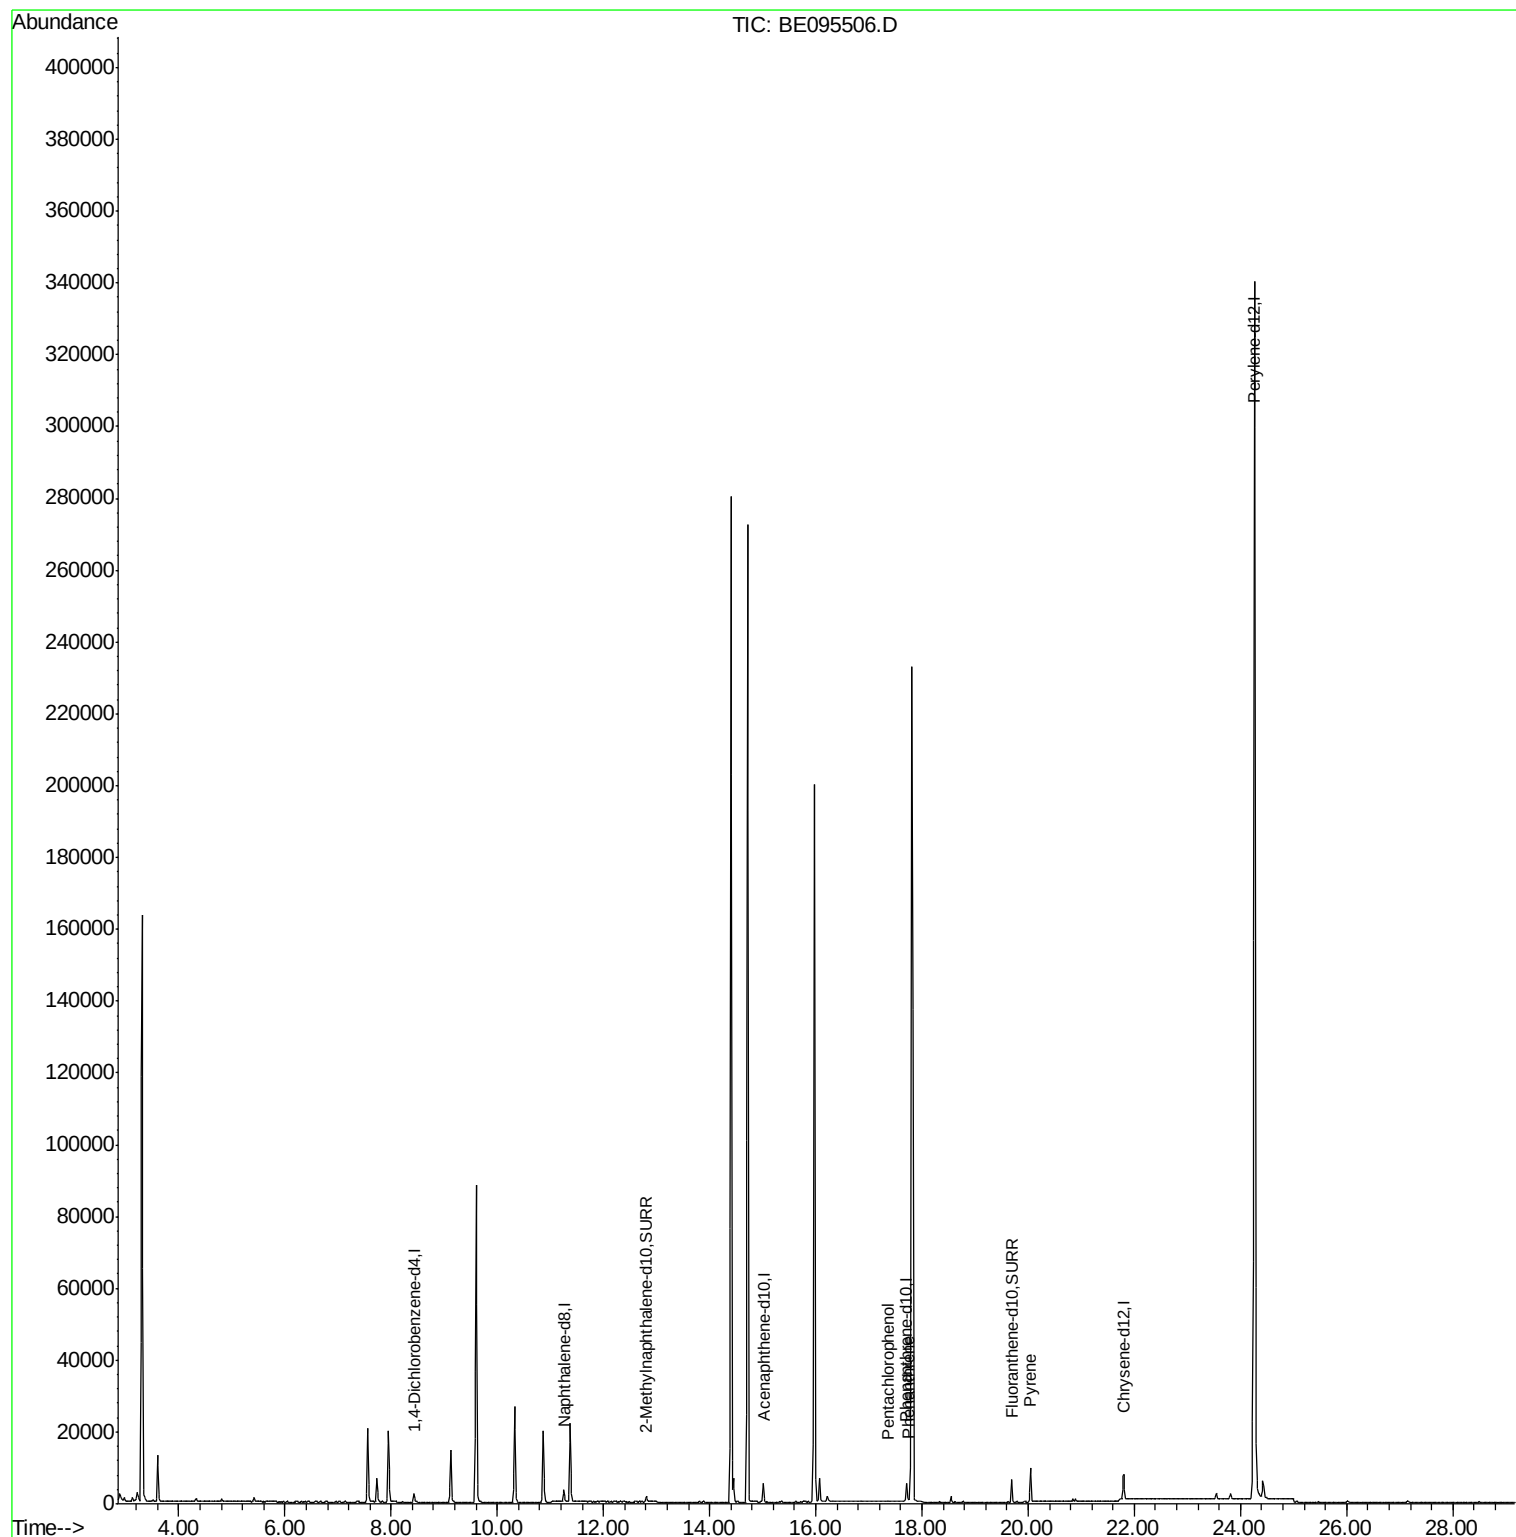


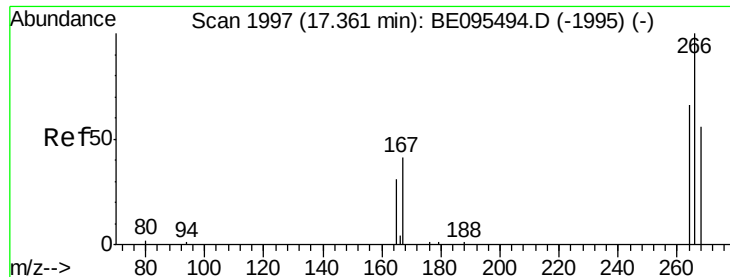

#11
 Pentachlorophenol
 Concen: 0.029 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095506.D
 Acq: 6 Feb 2018 00:21




Instrument :
 BNA_E
 ClientSampled :


Tot Ion:266 Resp: 39
 Ion Ratio Lower Upper
 266 100
 264 43.6 47.9 71.9#
 268 56.4 49.8 74.8

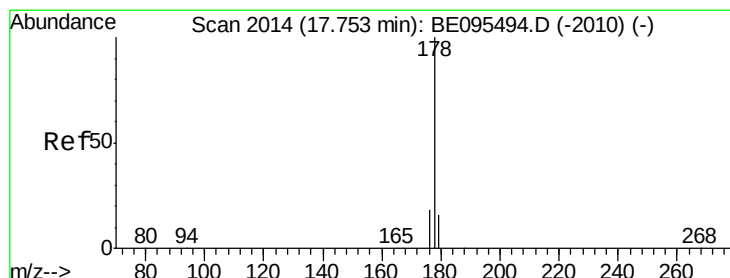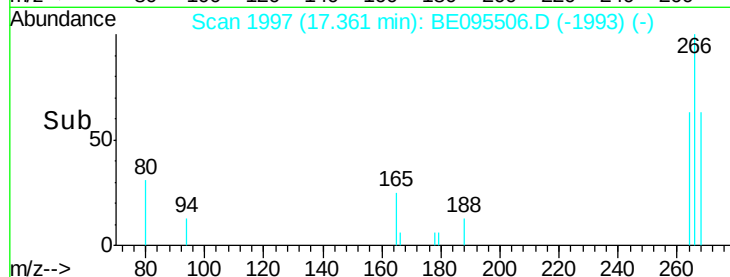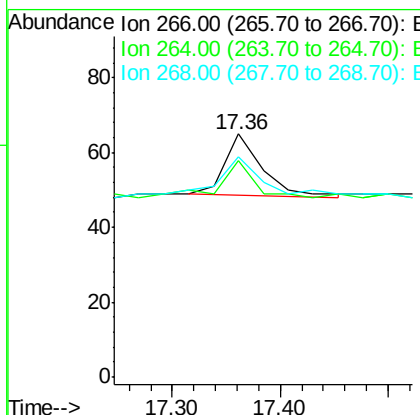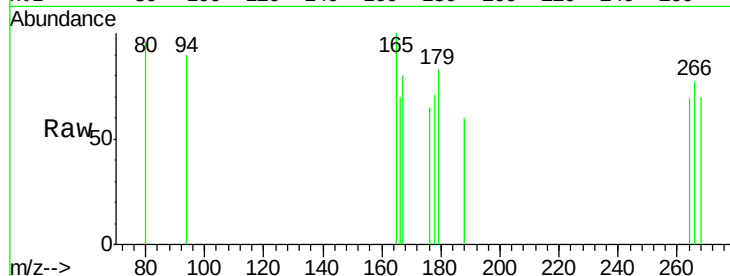

#12
 Phenanthrene
 Concen: 0.022 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. 0.00 min
 Lab File: BE095506.D
 Acq: 6 Feb 2018 00:21

Tgt Ion:178 Resp: 503
 Ion Ratio Lower Upper
 178 100
 179 48.8 18.4 27.6#
 176 39.8 13.6 20.4#

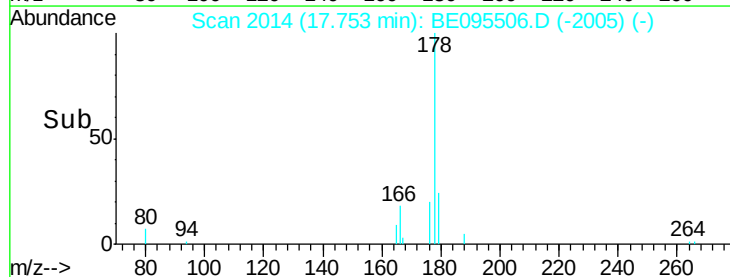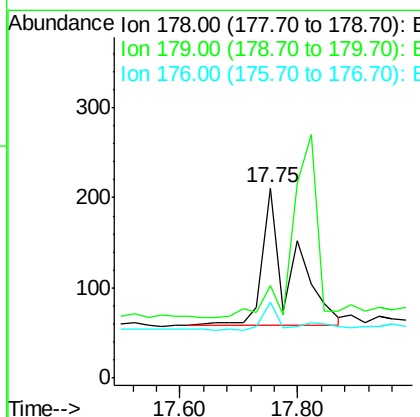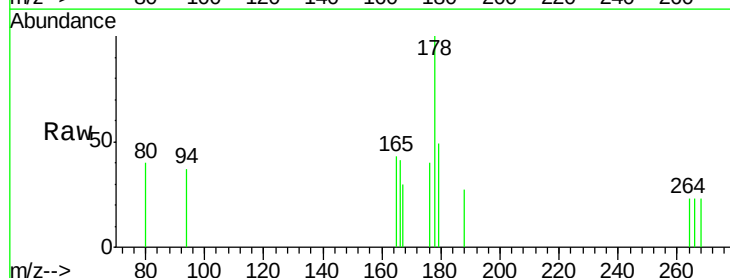

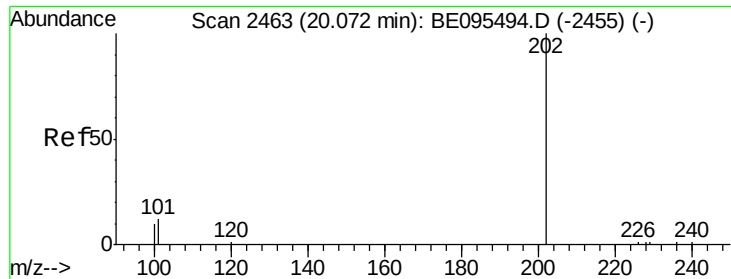

#17

Pvrene

Concen: 0.043 ng/ul

RT: 20.05 min Scan# 2459

Delta R.T. -0.03 min


Lab File: BE095506.D

Acq: 6 Feb 2018 00:21

Instrument :

BNA_E

ClientSampleId :

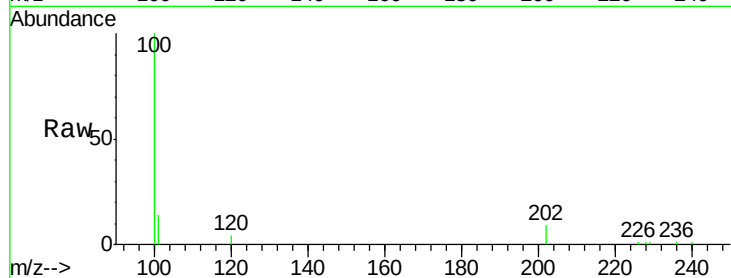

Tot Ion: 202 Resp: 1083

Ion Ratio Lower Upper

202 100

101 163.7 18.2 27.4#

100 1148.7 15.6 23.4#

