

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095507.D
 Acq On : 6 Feb 2018 00:56
 Operator : SJ/JU
 Sample : J1314-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 06 02:11:39 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 02:09:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1802	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5165	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3390	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7464	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7764	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	455081	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2717	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8197	0.29	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	130	0.090	ng/ul#	91
17) Pyrene	20.05	202	1397	0.054	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095507.D
Acq On : 6 Feb 2018 00:56
Operator : SJ/JU
Sample : J1314-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 06 02:11:39 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration

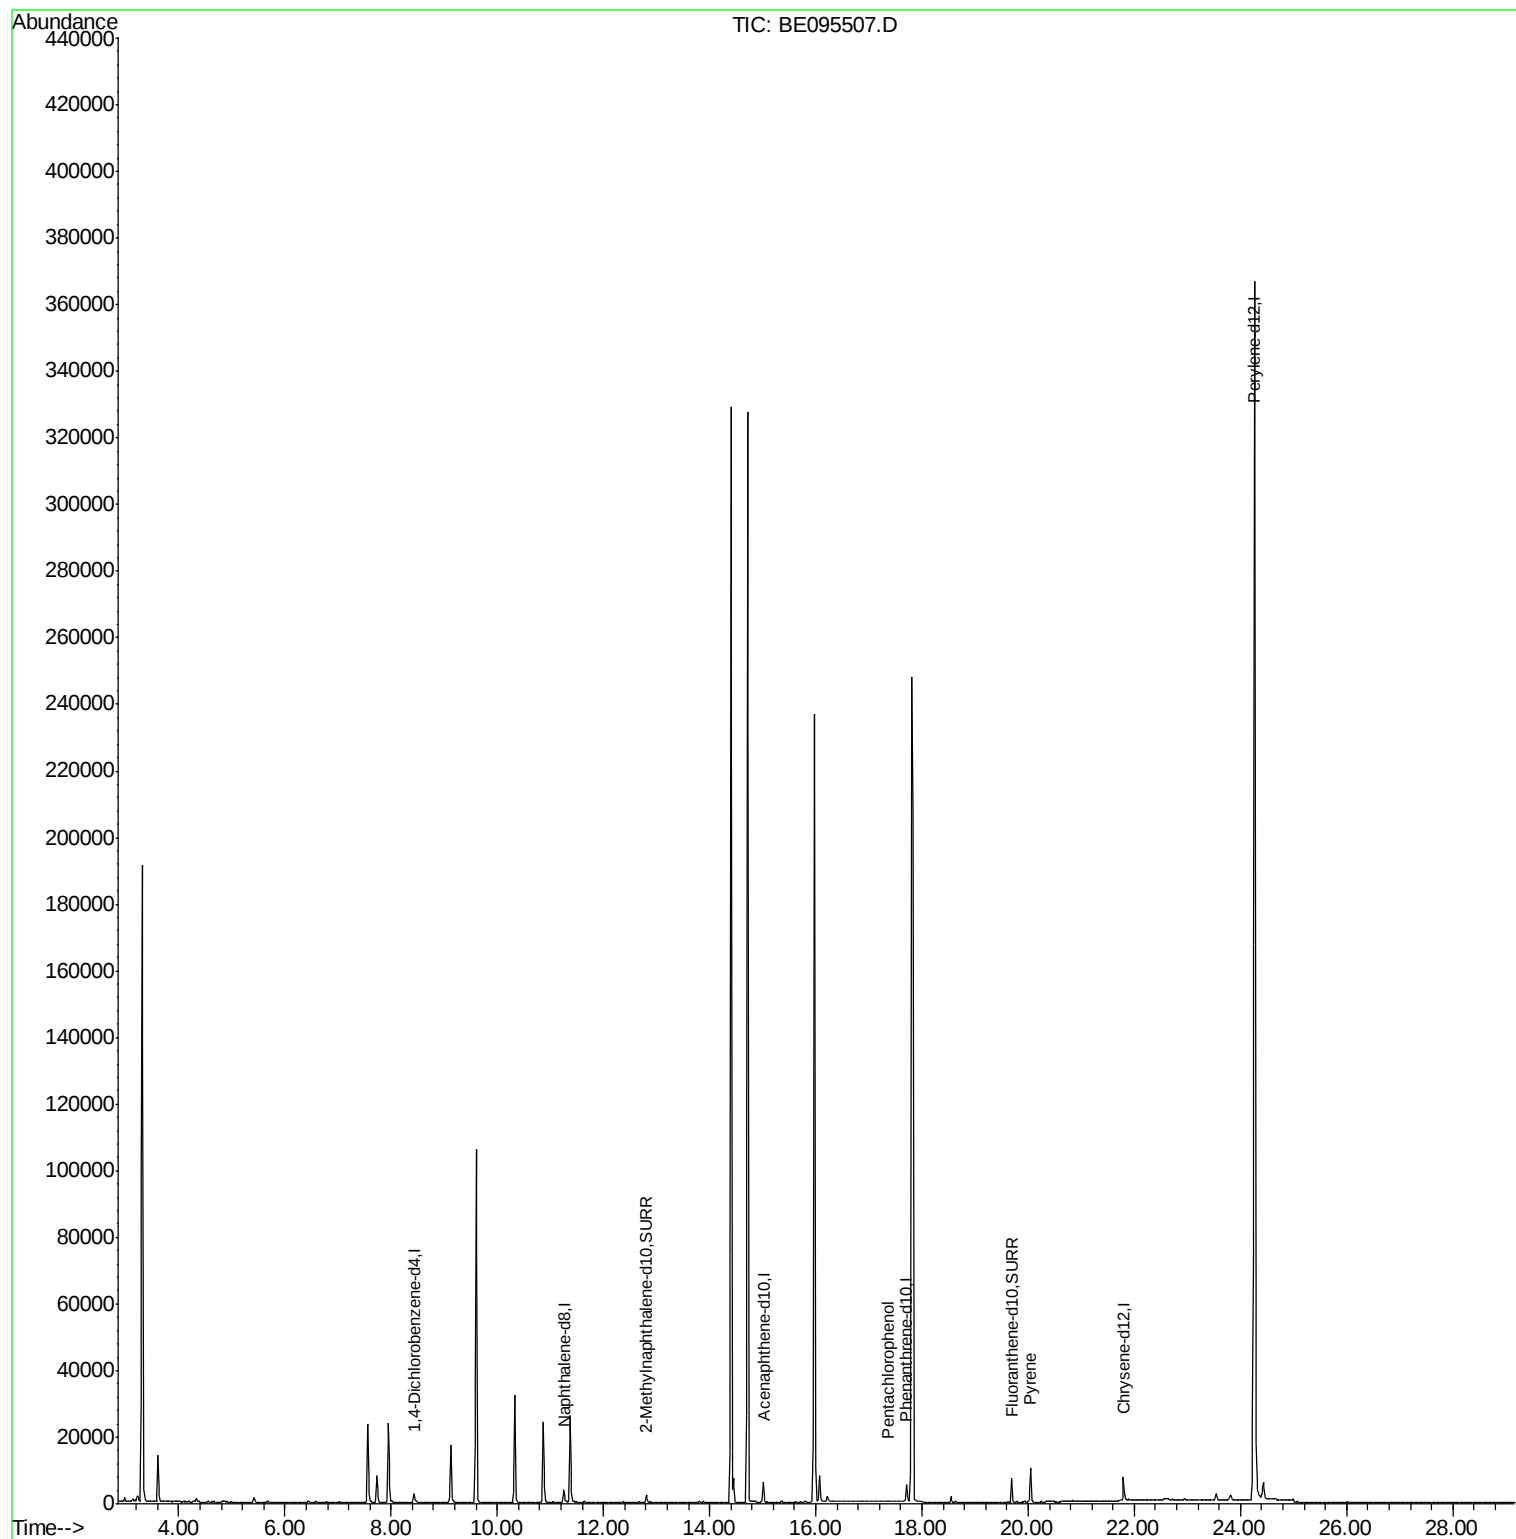


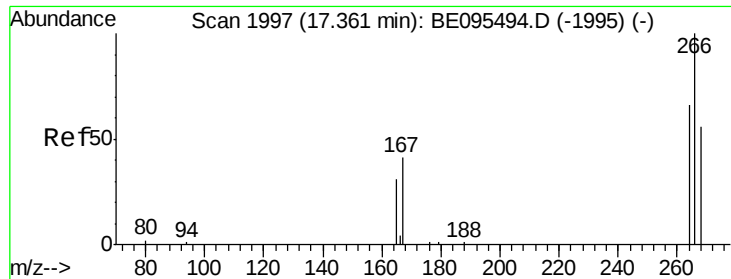




#11
 Pentachlorophenol
 Concen: 0.090 ng/ul
 RT: 17.36 min Scan# 1998
 Delta R.T. 0.00 min
 Lab File: BE095507.D
 Acq: 6 Feb 2018 00:56

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:266 Resp: 130
 Ion Ratio Lower Upper
 266 100
 264 72.3 47.9 71.9#
 268 63.8 49.8 74.8

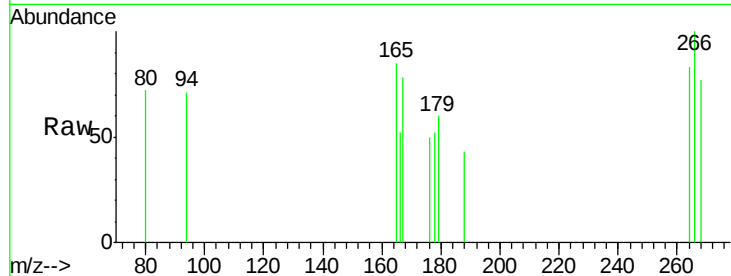


Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

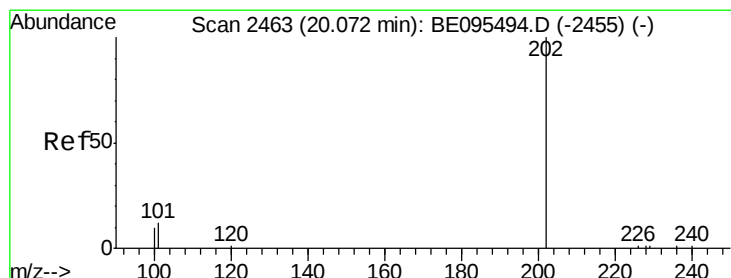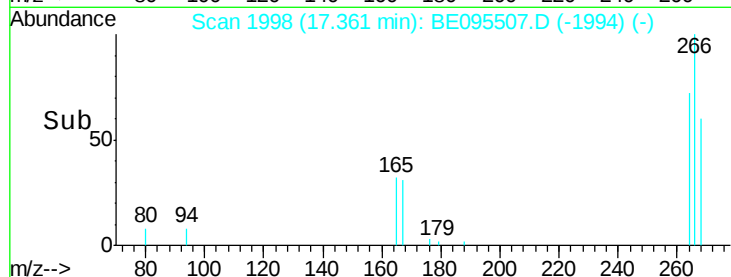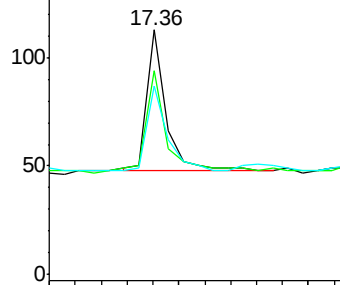

#17
 Pyrene
 Concen: 0.054 ng/ul
 RT: 20.05 min Scan# 2461
 Delta R.T. -0.02 min
 Lab File: BE095507.D
 Acq: 6 Feb 2018 00:56

Tgt Ion:202 Resp: 1397
 Ion Ratio Lower Upper
 202 100
 101 158.5 18.2 27.4#
 100 975.7 15.6 23.4#

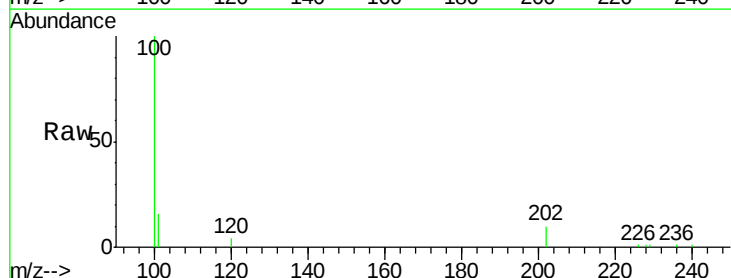

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): E

