

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095508.D
 Acq On : 6 Feb 2018 1:32
 Operator : SJ/JU
 Sample : J1314-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 06 02:11:45 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 02:09:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1673	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	4502	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3003	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6797	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6668	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	449865	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3233	0.44	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9769	0.38	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	17.36	266	82	0.062	ng/ul	97
12) Phenanthrene	17.75	178	766	0.034	ng/ul#	68
17) Pyrene	20.05	202	1492	0.067	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095508.D
Acq On : 6 Feb 2018 1:32
Operator : SJ/JU
Sample : J1314-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 06 02:11:45 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration




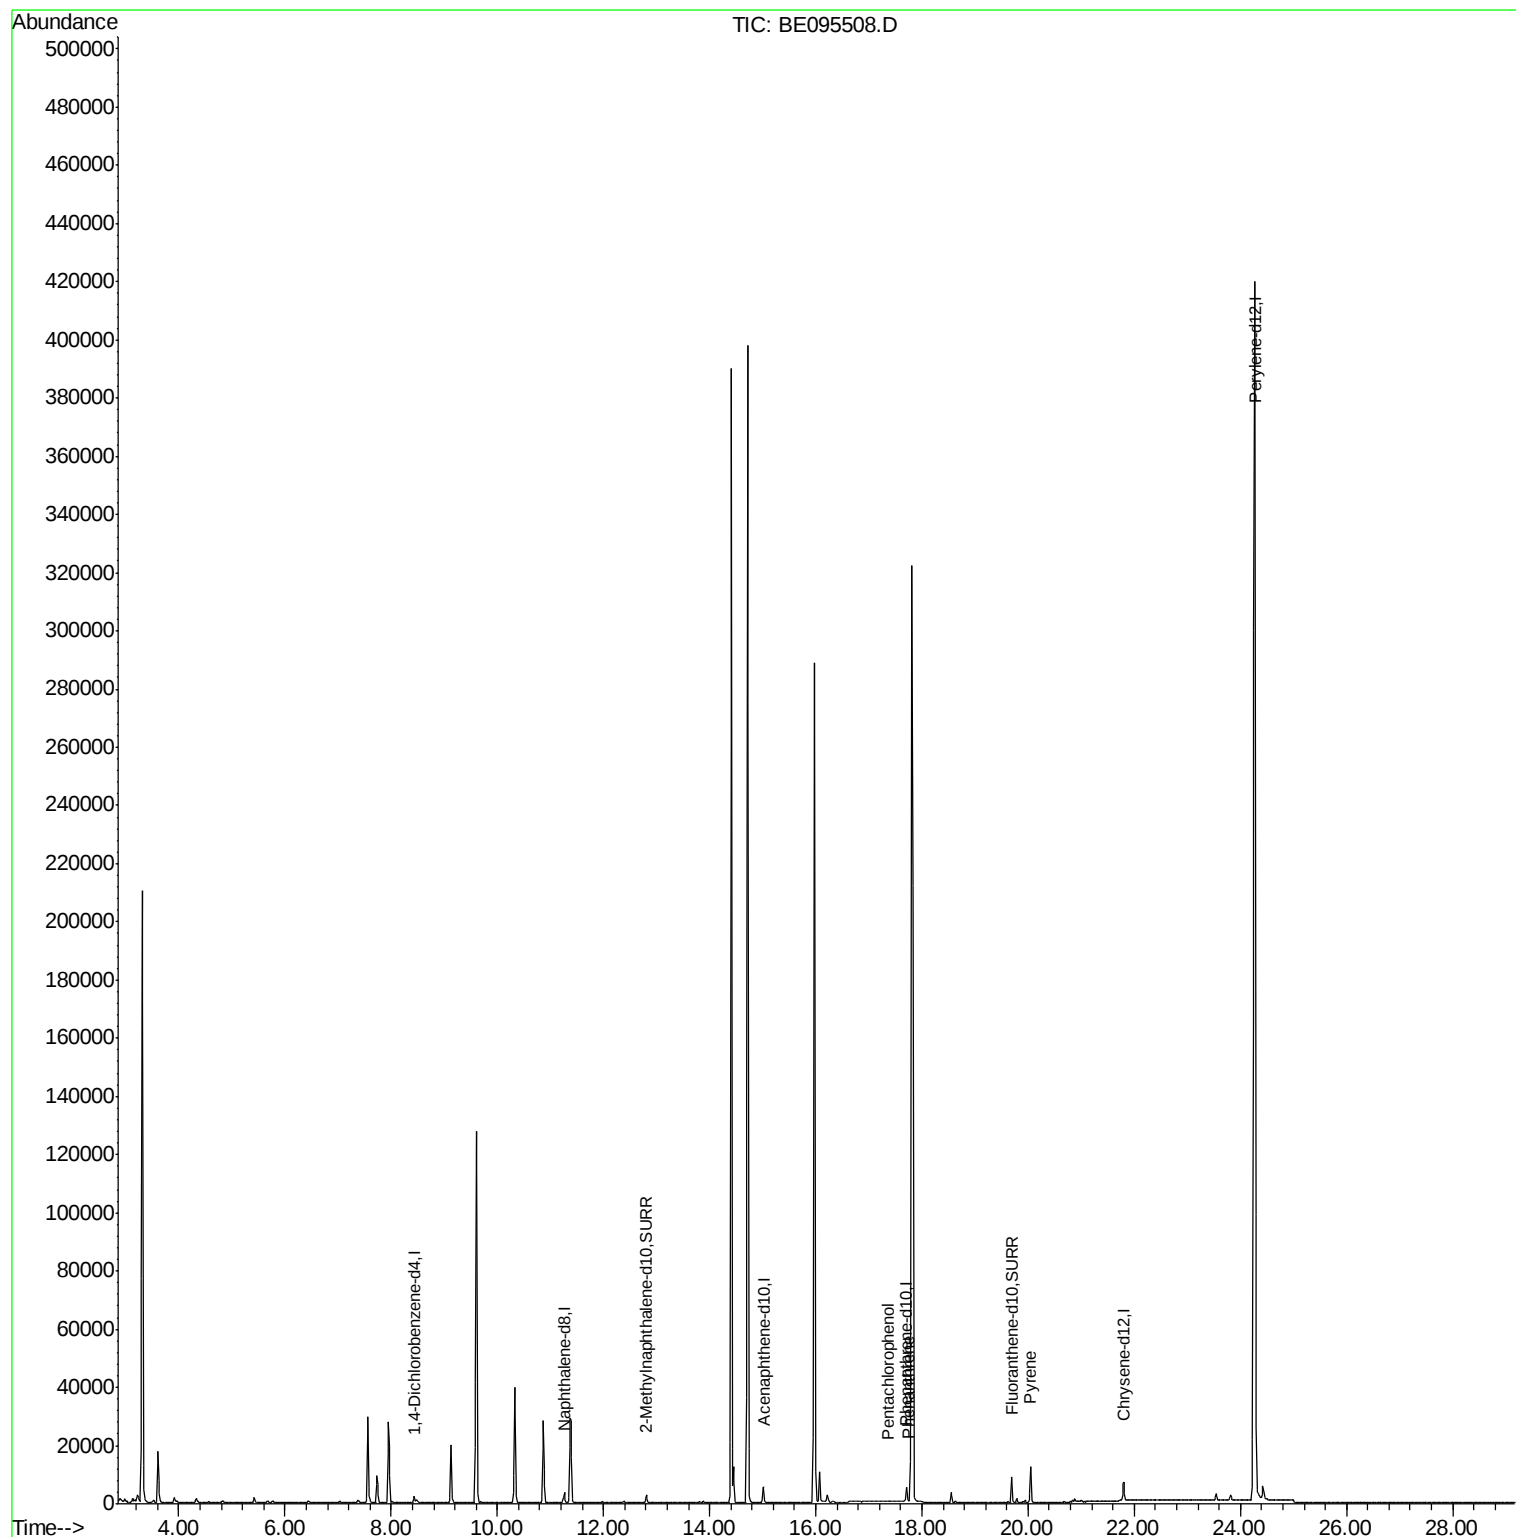


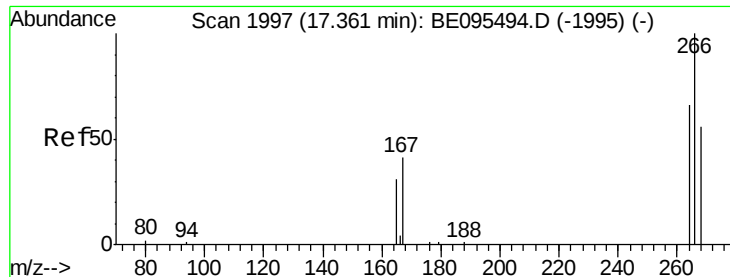

#11
 Pentachlorophenol
 Concen: 0.062 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095508.D
 Acq: 6 Feb 2018 1:32




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 82
 Ion Ratio Lower Upper
 266 100
 264 64.6 47.9 71.9
 268 62.2 49.8 74.8

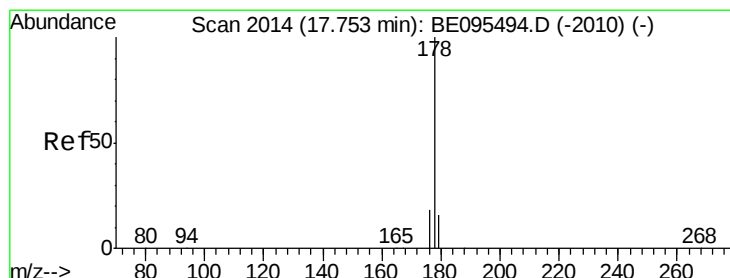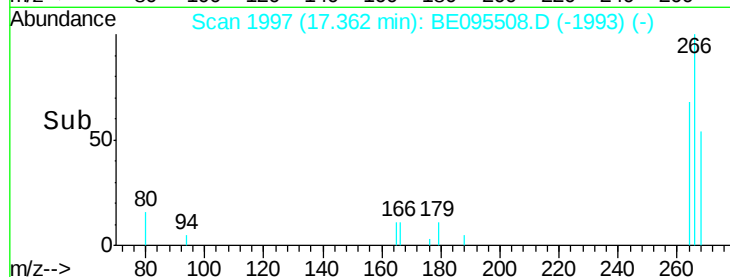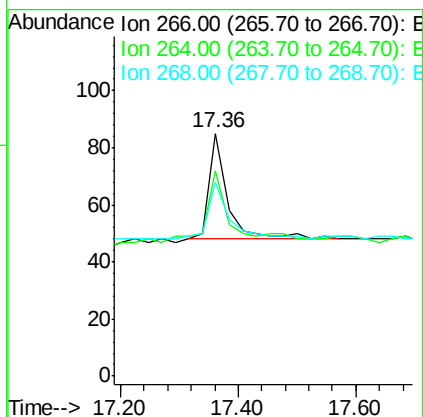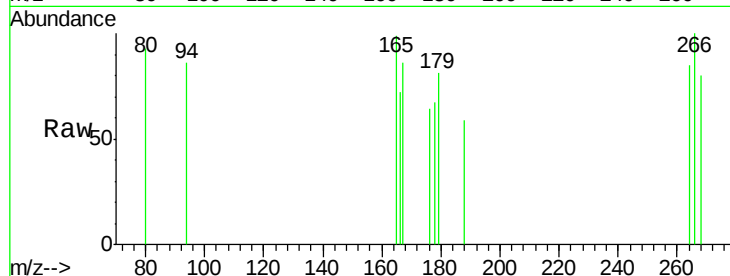

#12
 Phenanthrene
 Concen: 0.034 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. 0.00 min
 Lab File: BE095508.D
 Acq: 6 Feb 2018 1:32

Tgt Ion:178 Resp: 766
 Ion Ratio Lower Upper
 178 100
 179 38.0 18.4 27.6#
 176 31.3 13.6 20.4#

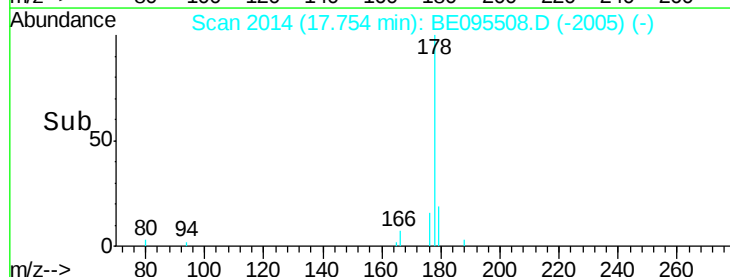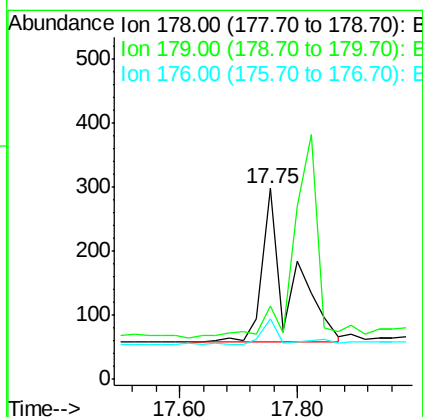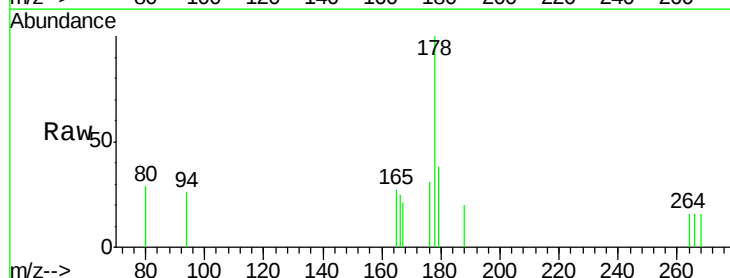


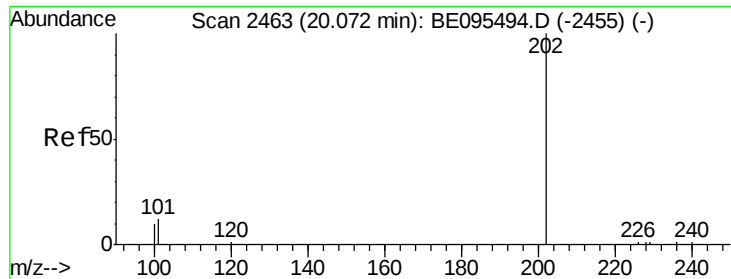

#17
 Pvrene
 Concen: 0.067 ng/ul
 RT: 20.05 min Scan# 2460
 Delta R.T. -0.02 min
 Lab File: BE095508.D
 Acq: 6 Feb 2018 1:32

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion: 202 Resp: 1492
 Ion Ratio Lower Upper
 202 100
 101 165.5 18.2 27.4#
 100 1026.4 15.6 23.4#

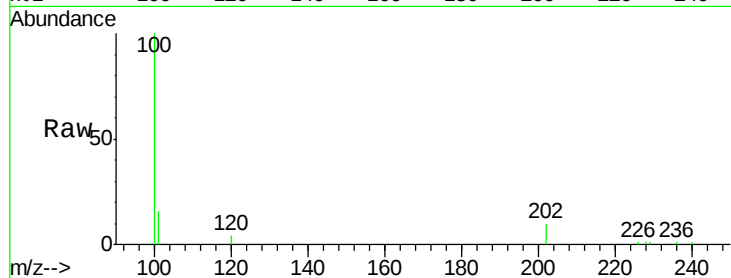

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): BE

