

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095513.D
 Acq On : 6 Feb 2018 4:31
 Operator : SJ/JU
 Sample : J1315-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 06 05:56:28 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 04:22:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1700	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	4703	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3014	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7022	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6985	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	381410	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2381	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7044	0.26	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	17.36	266	160	0.118	ng/ul	90
12) Phenanthrene	17.75	178	556	0.024	ng/ul#	59
17) Pyrene	20.04	202	1141	0.049	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095513.D
Acq On : 6 Feb 2018 4:31
Operator : SJ/JU
Sample : J1315-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 06 05:56:28 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

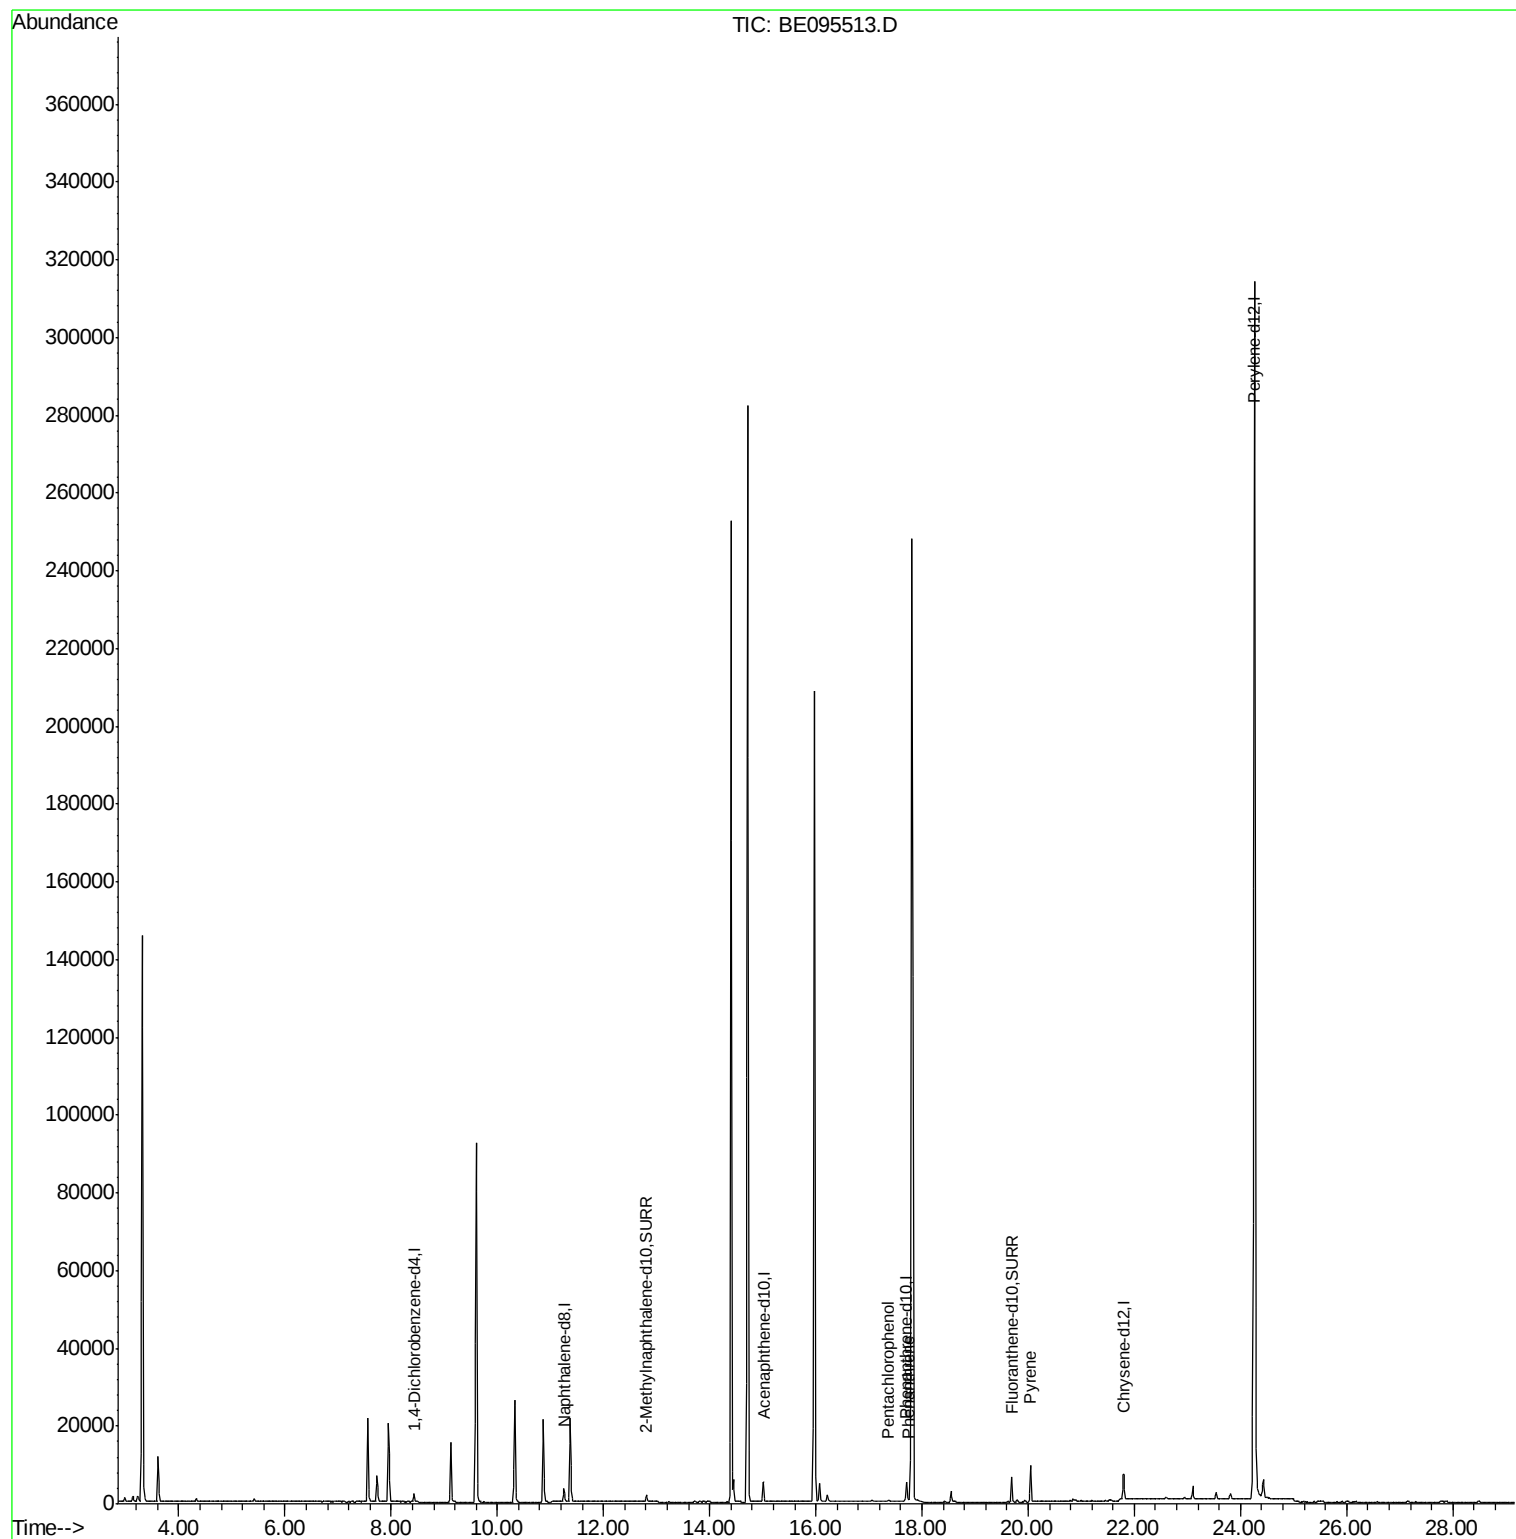


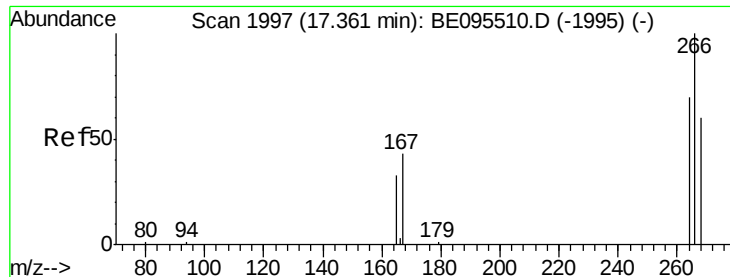


#11
 Pentachlorophenol
 Concen: 0.118 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095513.D
 Acq: 6 Feb 2018 4:31

Instrument :
 BNA_E
 ClientSampleId :



Tot Ion:266 Resp: 160
 Ion Ratio Lower Upper
 266 100
 264 65.0 47.9 71.9
 268 71.9 49.8 74.8

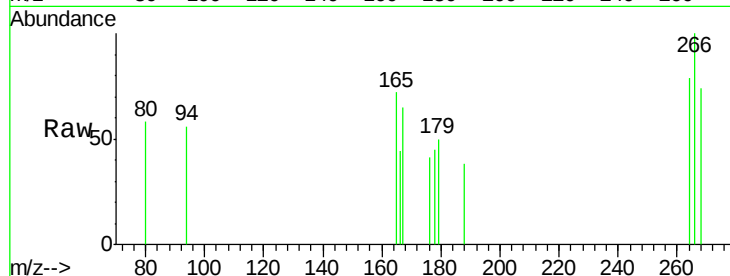

Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

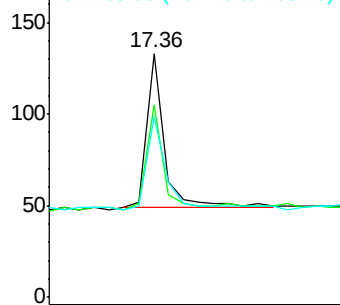


Time-->

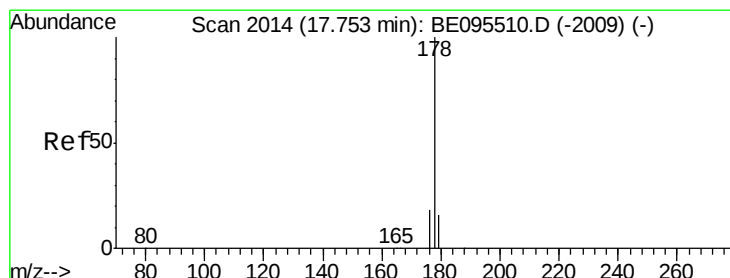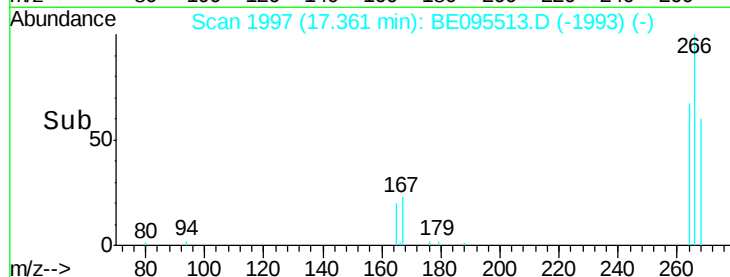


#12
 Phenanthrene
 Concen: 0.024 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. 0.00 min
 Lab File: BE095513.D
 Acq: 6 Feb 2018 4:31


Tgt Ion:178 Resp: 556
 Ion Ratio Lower Upper
 178 100
 179 41.7 18.4 27.6#
 176 36.4 13.6 20.4#



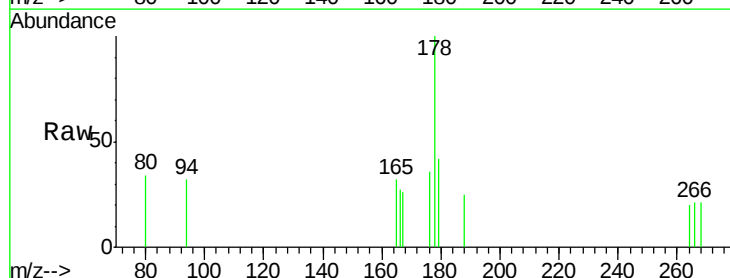


Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

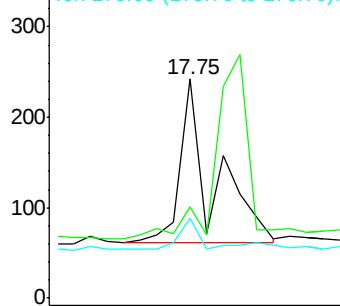

Time-->

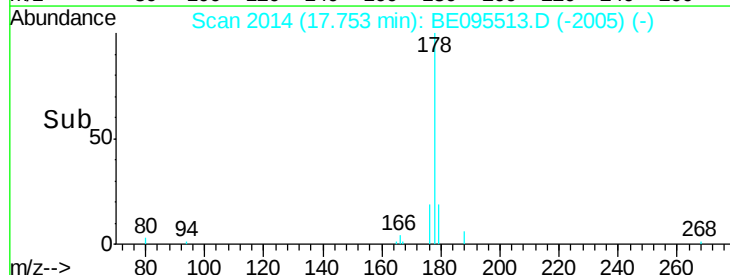

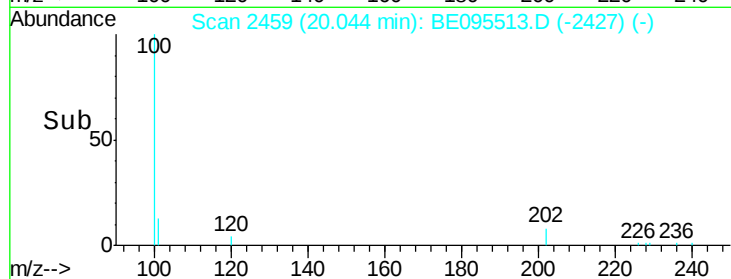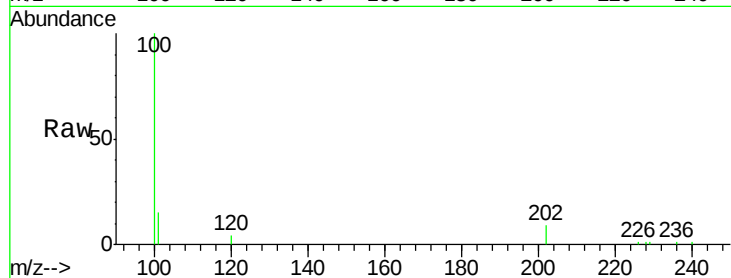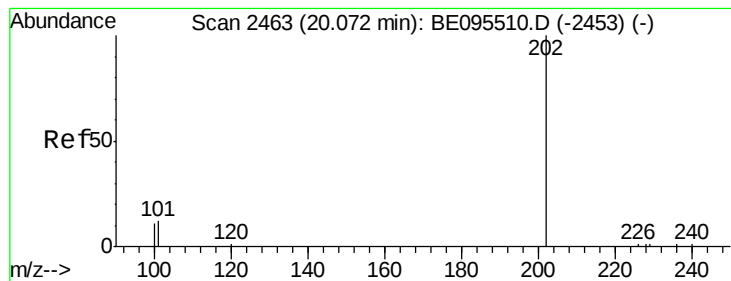

#17

Pvrene

Concen: 0.049 ng/ul

RT: 20.04 min Scan# 2459

Delta R.T. -0.03 min

Lab File: BE095513.D

Acq: 6 Feb 2018 4:31

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 202 Resp: 1141

Ion Ratio Lower Upper

202 100

101 164.4 18.2 27.4#

100 1119.7 15.6 23.4#

