

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095515.D
 Acq On : 6 Feb 2018 5:43
 Operator : SJ/JU
 Sample : J1315-12
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 06 06:30:19 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 04:22:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1872	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5373	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3463	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8116	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8062	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	567447	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3379	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9978	0.32	ng/ul	0.00
Target Compounds						
17) Pyrene	20.05	202	1503	0.056	ng/ul#	Ovalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095515.D
Acq On : 6 Feb 2018 5:43
Operator : SJ/JU
Sample : J1315-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 06 06:30:19 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

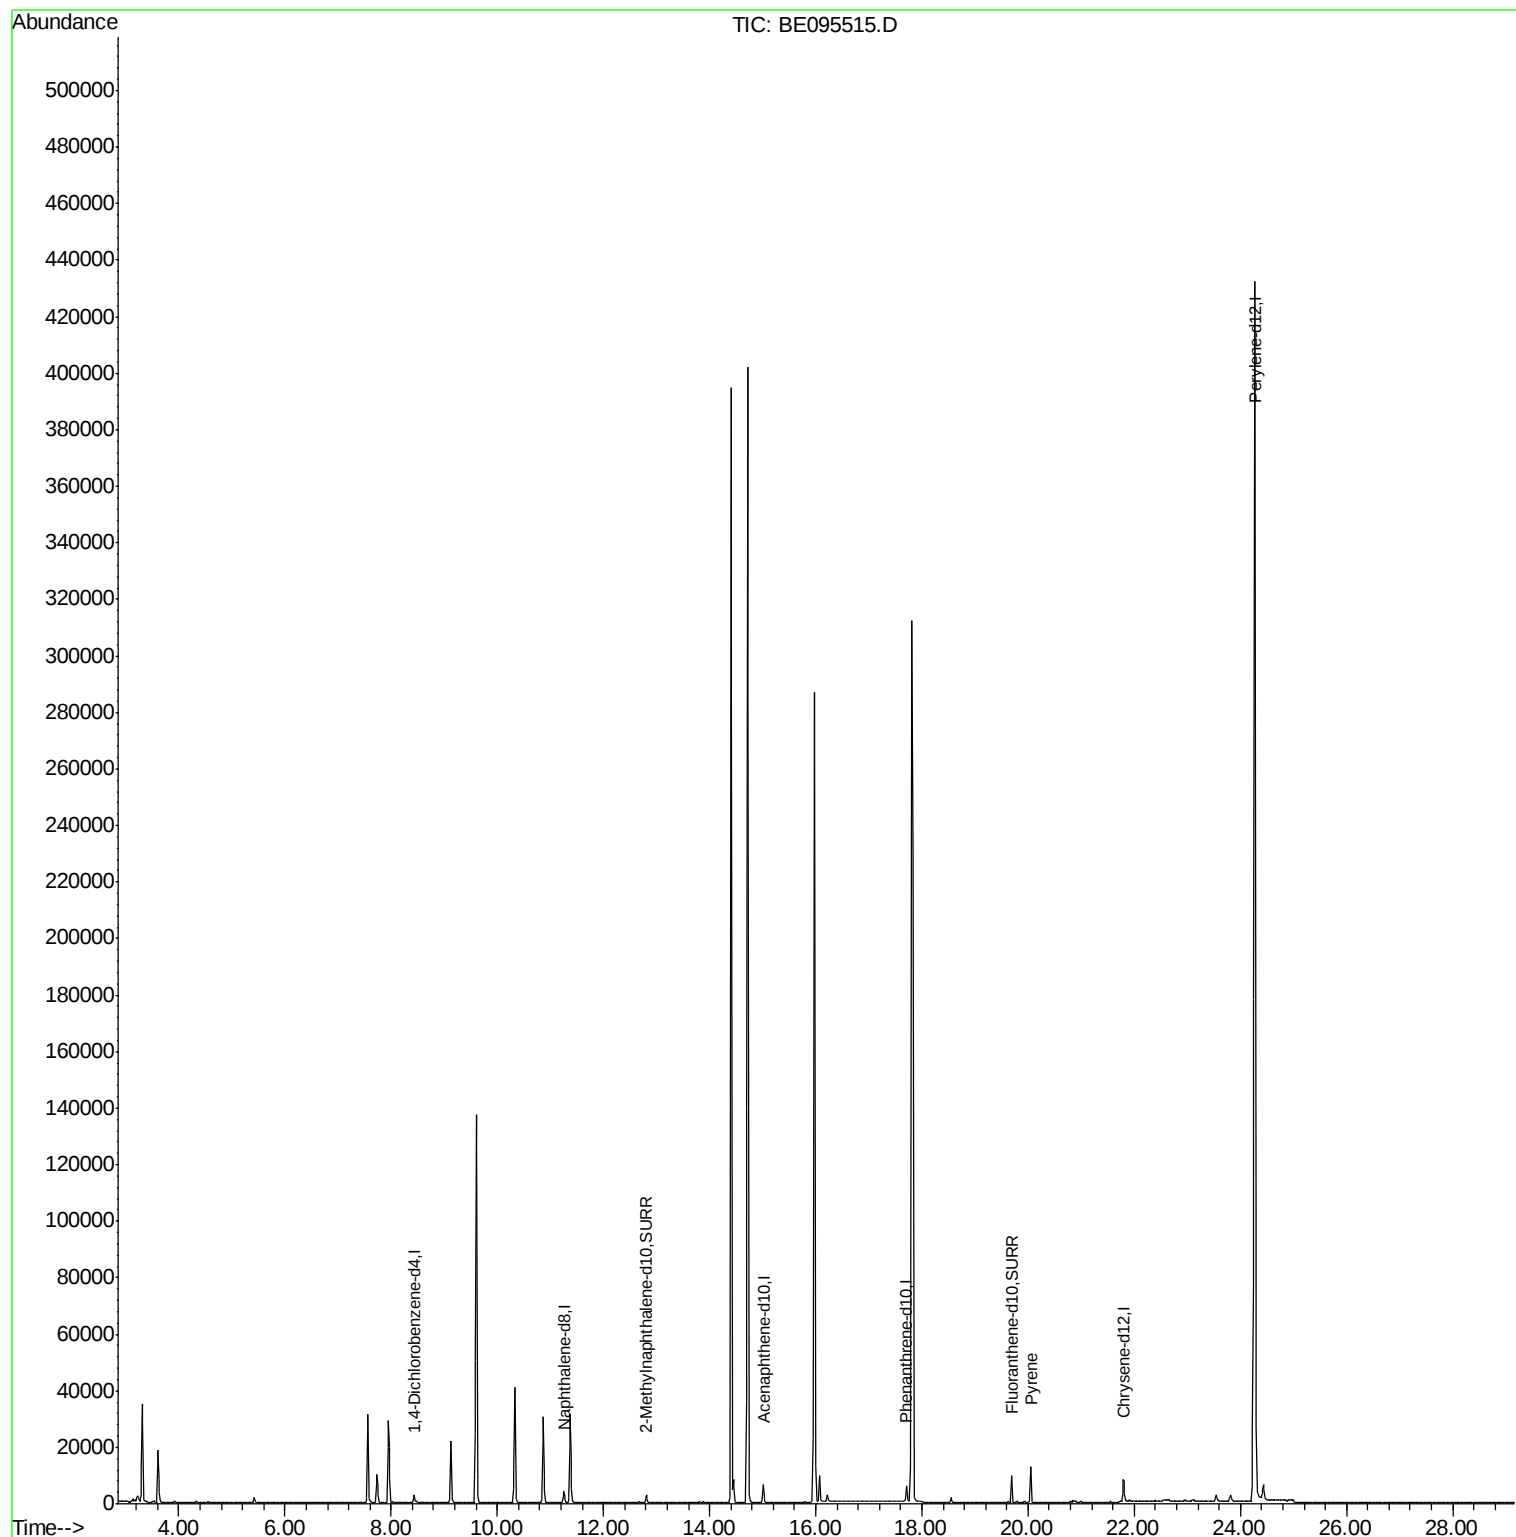

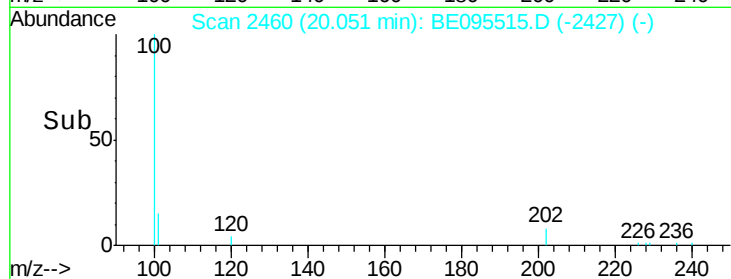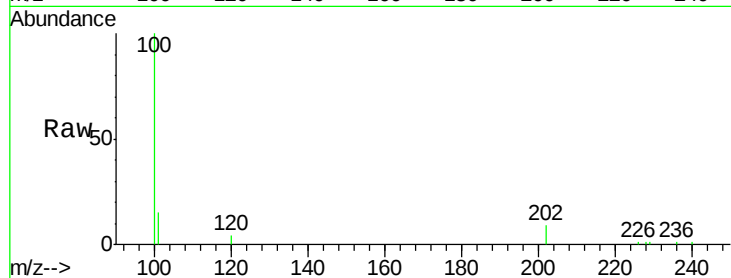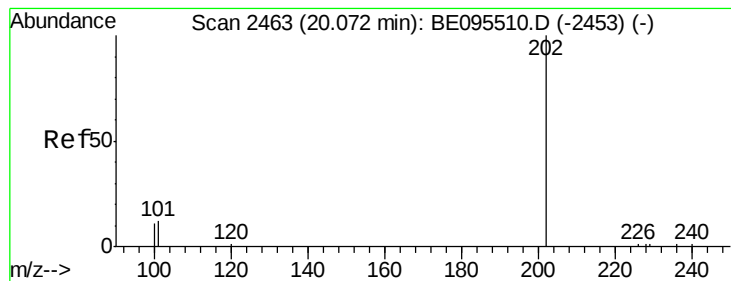

#17

Pvrene

Concen: 0.056 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.02 min

Lab File: BE095515.D

Acq: 6 Feb 2018 5:43

Instrument :

BNA_E

ClientSampleId :

Tot Ion:202 Resp: 1503

Ion Ratio Lower Upper

202 100

101 171.0 18.2 27.4#

100 1104.0 15.6 23.4#

