

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095520.D
Acq On : 6 Feb 2018 8:39
Operator : SJ/JU
Sample : PB106191BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK91

Quant Time: Feb 06 10:41:02 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1936	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5526	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3537	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8340	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8212	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	628996	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3143	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9616	0.30	ng/ul	0.00
Target Compounds						
17) Pyrene	20.05	202	1406	0.051	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095520.D
Acq On : 6 Feb 2018 8:39
Operator : SJ/JU
Sample : PB106191BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK91

Quant Time: Feb 06 10:41:02 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

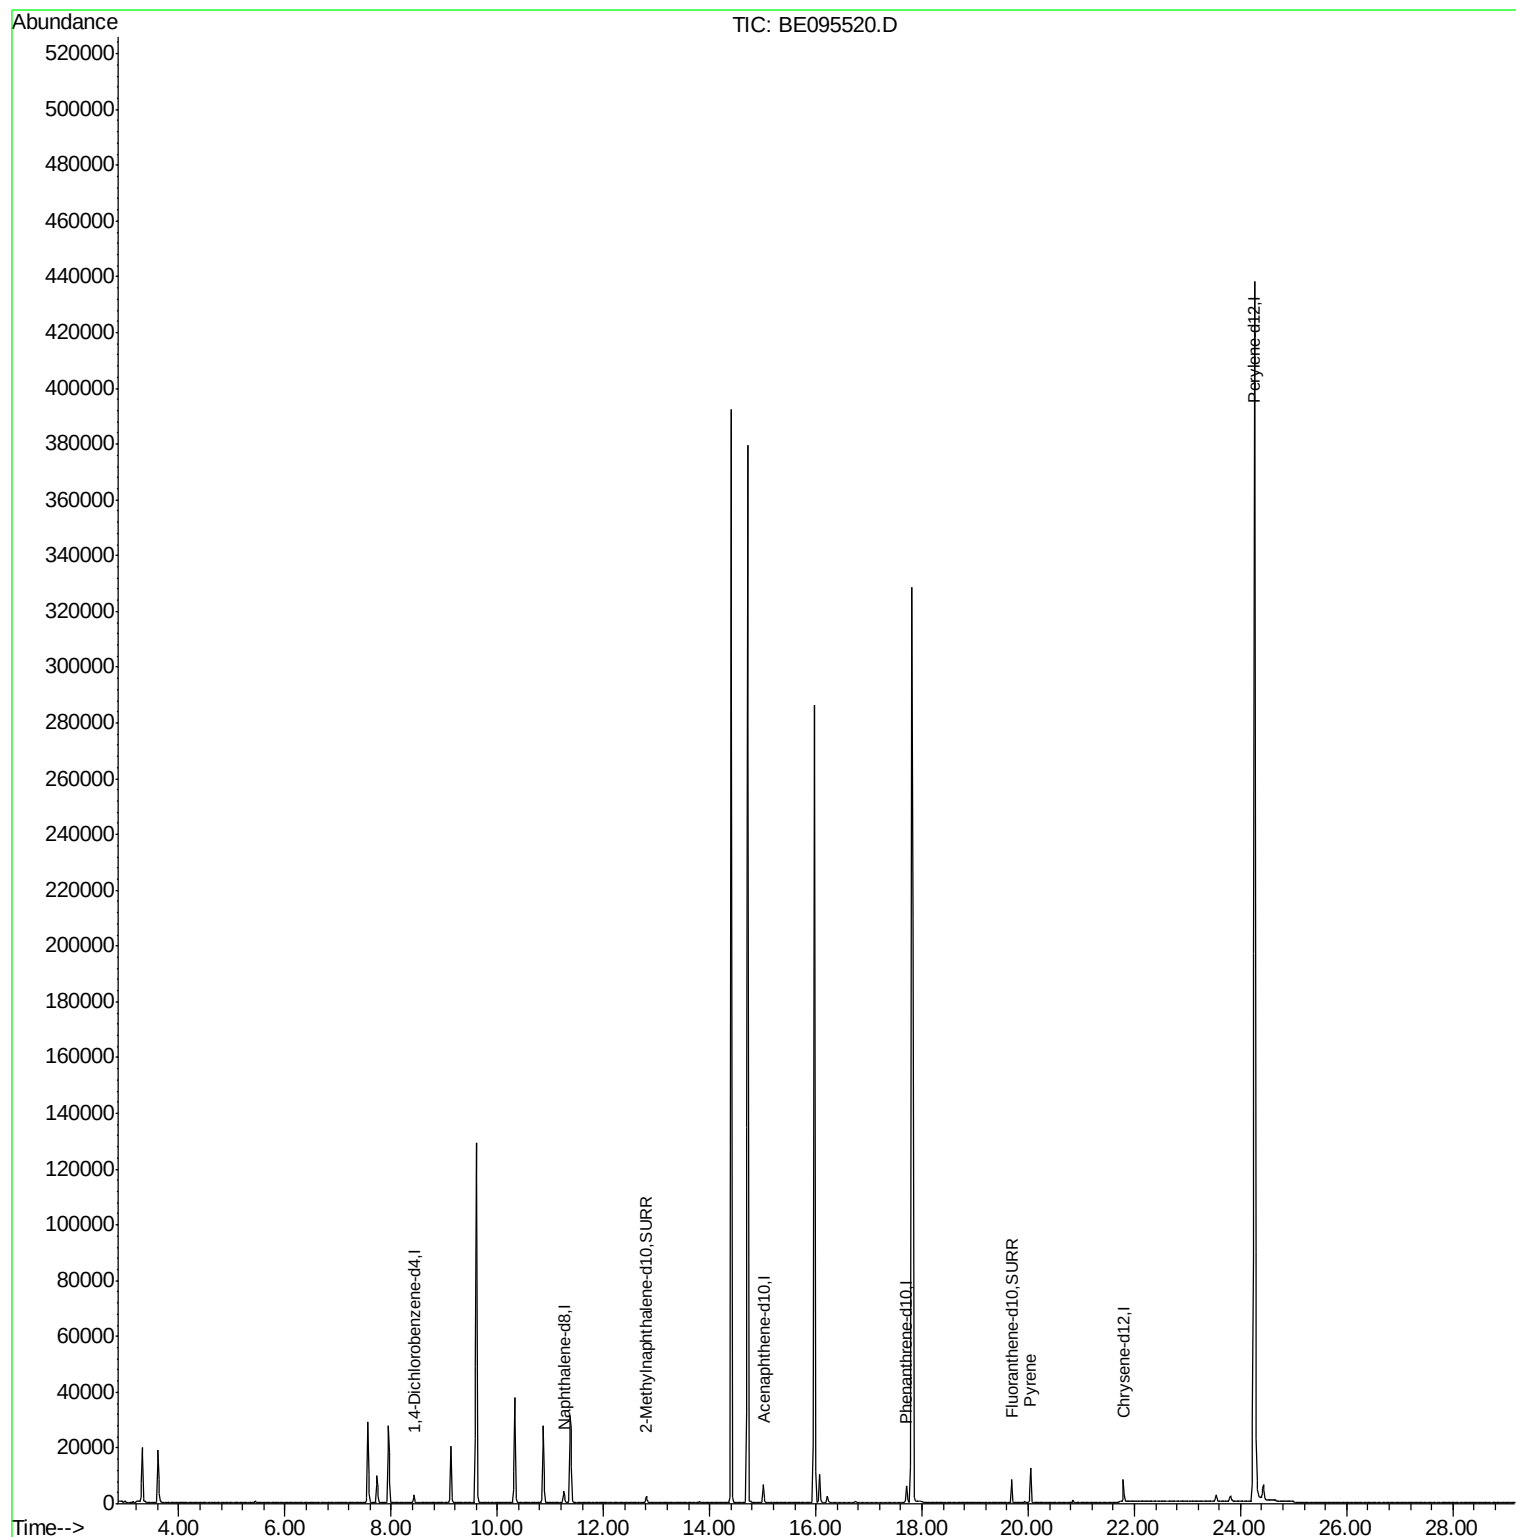

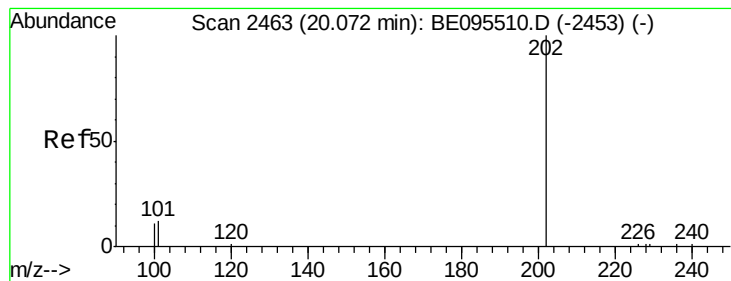

#17

Pyrene

Concen: 0.051 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.02 min

Lab File: BE095520.D

Acq: 6 Feb 2018 8:39

Instrument :

BNA_E

ClientSampleId :

SBLK91


Tgt Ion: 202 Resp: 1406

Ion Ratio Lower Upper

202 100

101 168.3 18.2 27.4#

100 1052.5 15.6 23.4#

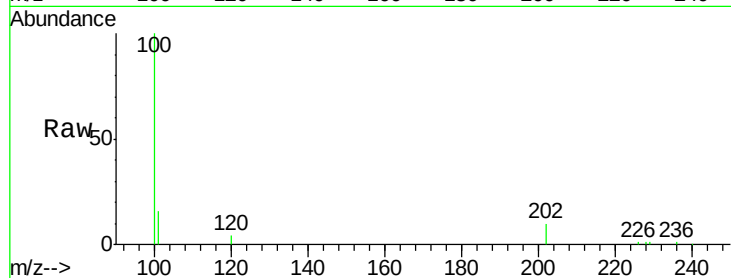

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

