

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
 Data File : BE095521.D
 Acq On : 6 Feb 2018 9:15
 Operator : SJ/JU
 Sample : J1316-16
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C96

Quant Time: Feb 06 10:41:07 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 04:22:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1935	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5705	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3630	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8163	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8302	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	496003	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2717	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7988	0.26	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	50	0.032	ng/ul	96
17) Pyrene	20.05	202	1358	0.049	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095521.D
Acq On : 6 Feb 2018 9:15
Operator : SJ/JU
Sample : J1316-16
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C96

Quant Time: Feb 06 10:41:07 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration




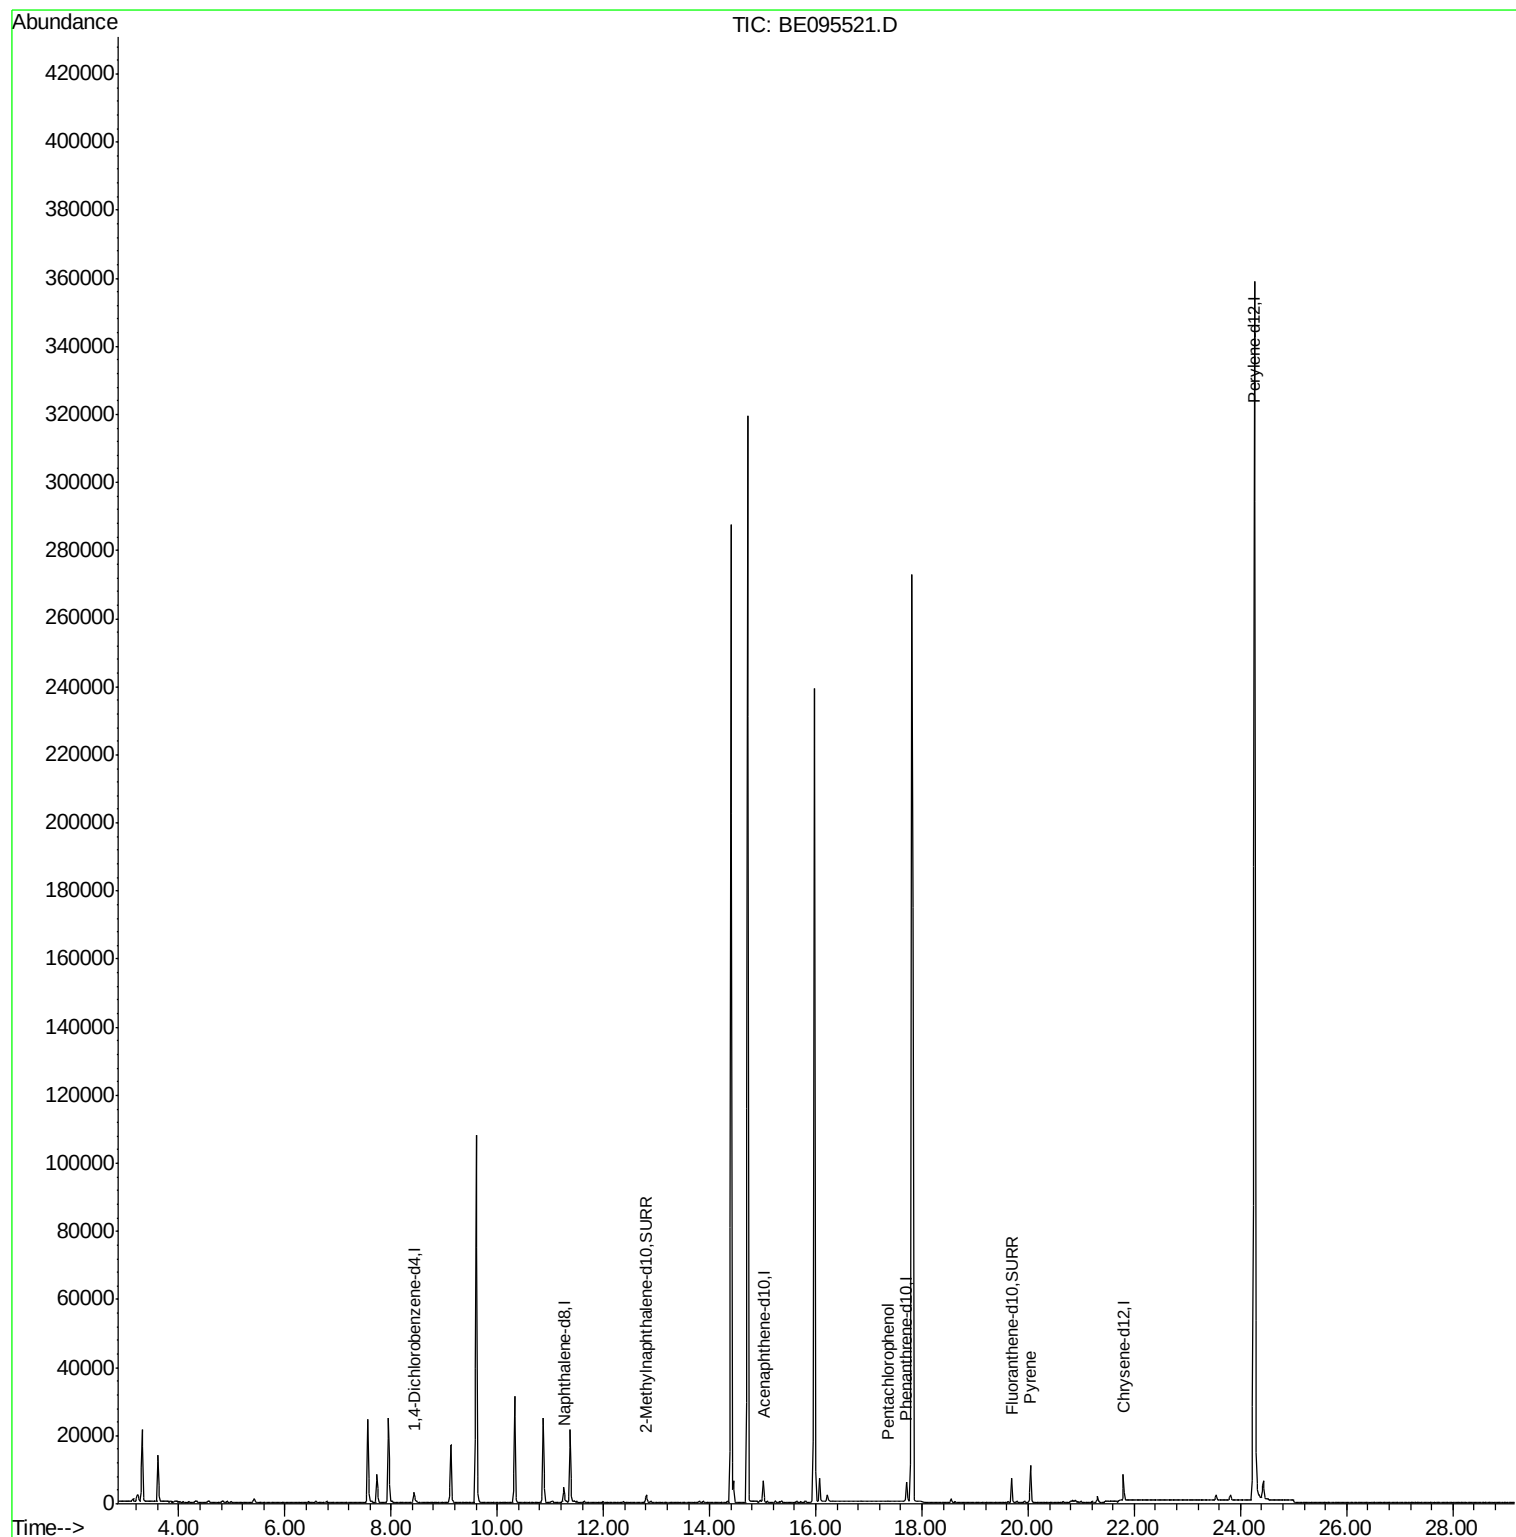


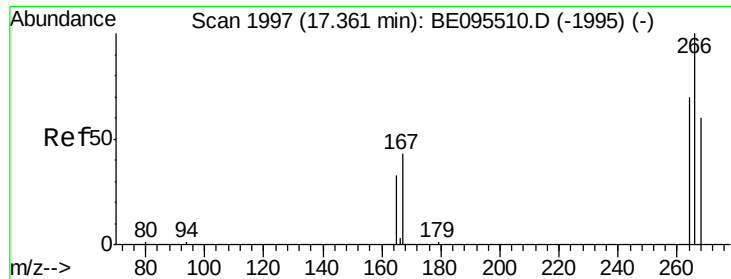

#11
 Pentachlorophenol
 Concen: 0.032 ng/ul
 RT: 17.36 min Scan# 1998
 Delta R.T. -0.00 min
 Lab File: BE095521.D
 Acq: 6 Feb 2018 9:15

Instrument :
 BNA_E
 ClientSampleId :
 F6C96

Tgt Ion: 266 Resp: 50
 Ion Ratio Lower Upper
 266 100
 264 58.0 47.9 71.9
 268 66.0 49.8 74.8

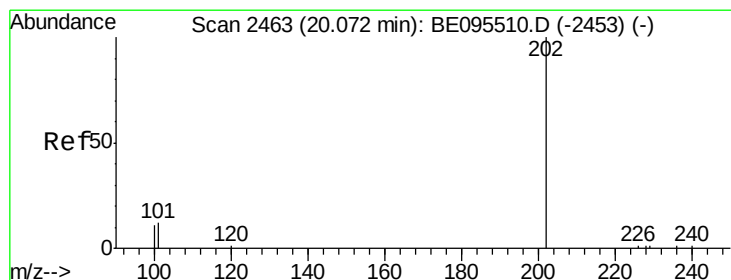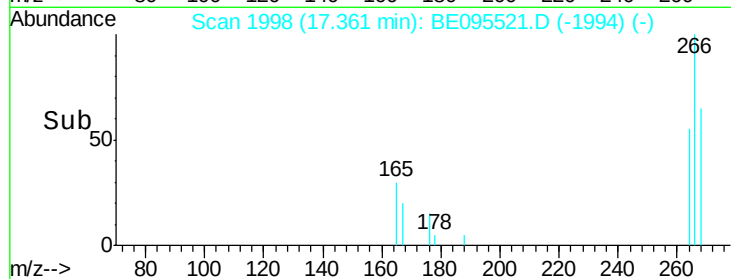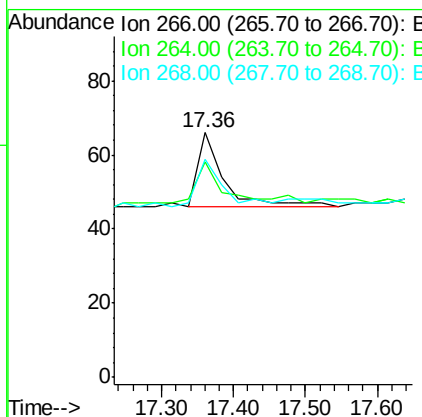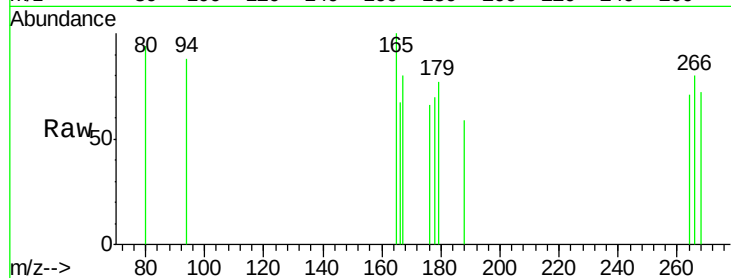

#17
 Pyrene
 Concen: 0.049 ng/ul
 RT: 20.05 min Scan# 2460
 Delta R.T. -0.03 min
 Lab File: BE095521.D
 Acq: 6 Feb 2018 9:15

Tgt Ion: 202 Resp: 1358
 Ion Ratio Lower Upper
 202 100
 101 168.3 18.2 27.4#
 100 1194.1 15.6 23.4#

