

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095523.D
Acq On : 6 Feb 2018 10:26
Operator : SJ/JU
Sample : J1316-15
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D38

Quant Time: Feb 06 11:05:48 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1781	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5024	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3215	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7574	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7324	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	427462	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2594	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7699	0.27	ng/ul	0.00
Target Compounds						
17) Pyrene	20.04	202	1118	0.045	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095523.D
Acq On : 6 Feb 2018 10:26
Operator : SJ/JU
Sample : J1316-15
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D38

Quant Time: Feb 06 11:05:48 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

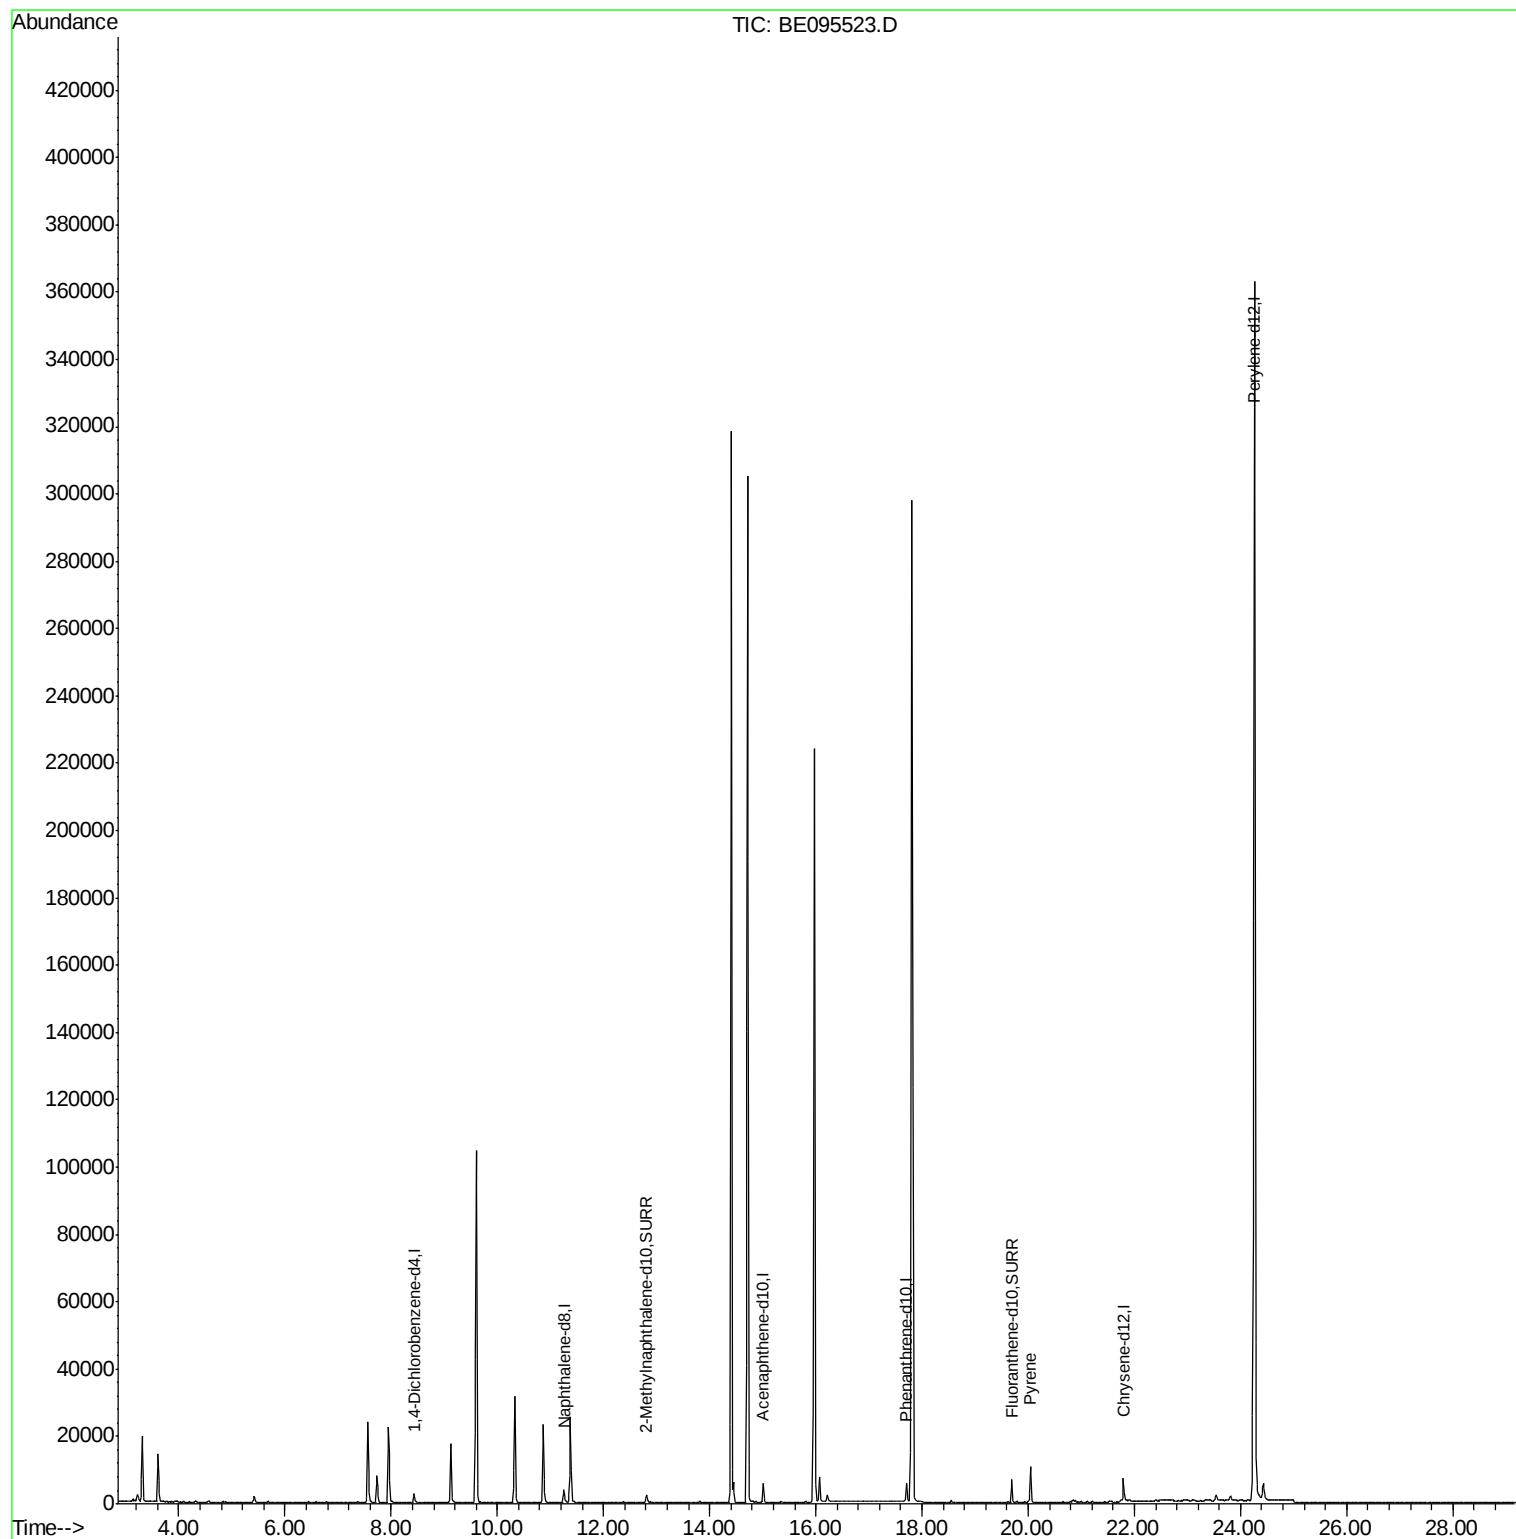

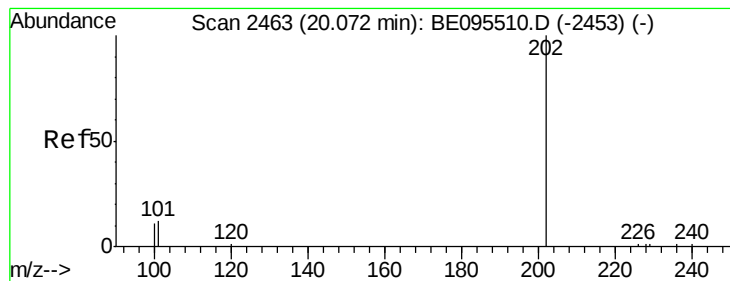

#17

Pyrene

Concen: 0.045 ng/ul

RT: 20.04 min Scan# 2459

Delta R.T. -0.03 min

Lab File: BE095523.D

Acq: 6 Feb 2018 10:26

Instrument :

BNA_E

ClientSampleId :

F6D38


Tgt Ion:202 Resp: 1118

Ion Ratio Lower Upper

202 100

101 172.0 18.2 27.4#

100 1228.4 15.6 23.4#

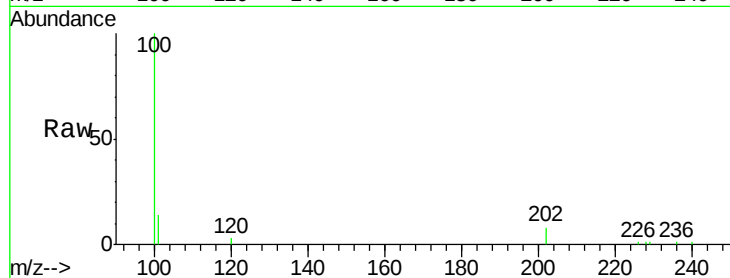

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

