

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
 Data File : BE095524.D
 Acq On : 6 Feb 2018 11:02
 Operator : SJ/JU
 Sample : J1296-05DL 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C23DL

Quant Time: Feb 06 12:23:06 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 04:22:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1716	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4760	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	2900	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7009	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7105	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7277	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	676	0.09	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	1896	0.07	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	789	0.581	ng/ul	98
23) Benzo(a)pyrene	24.26	252	554	0.024	ng/ul#	8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095524.D
Acq On : 6 Feb 2018 11:02
Operator : SJ/JU
Sample : J1296-05DL 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C23DL

Quant Time: Feb 06 12:23:06 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration




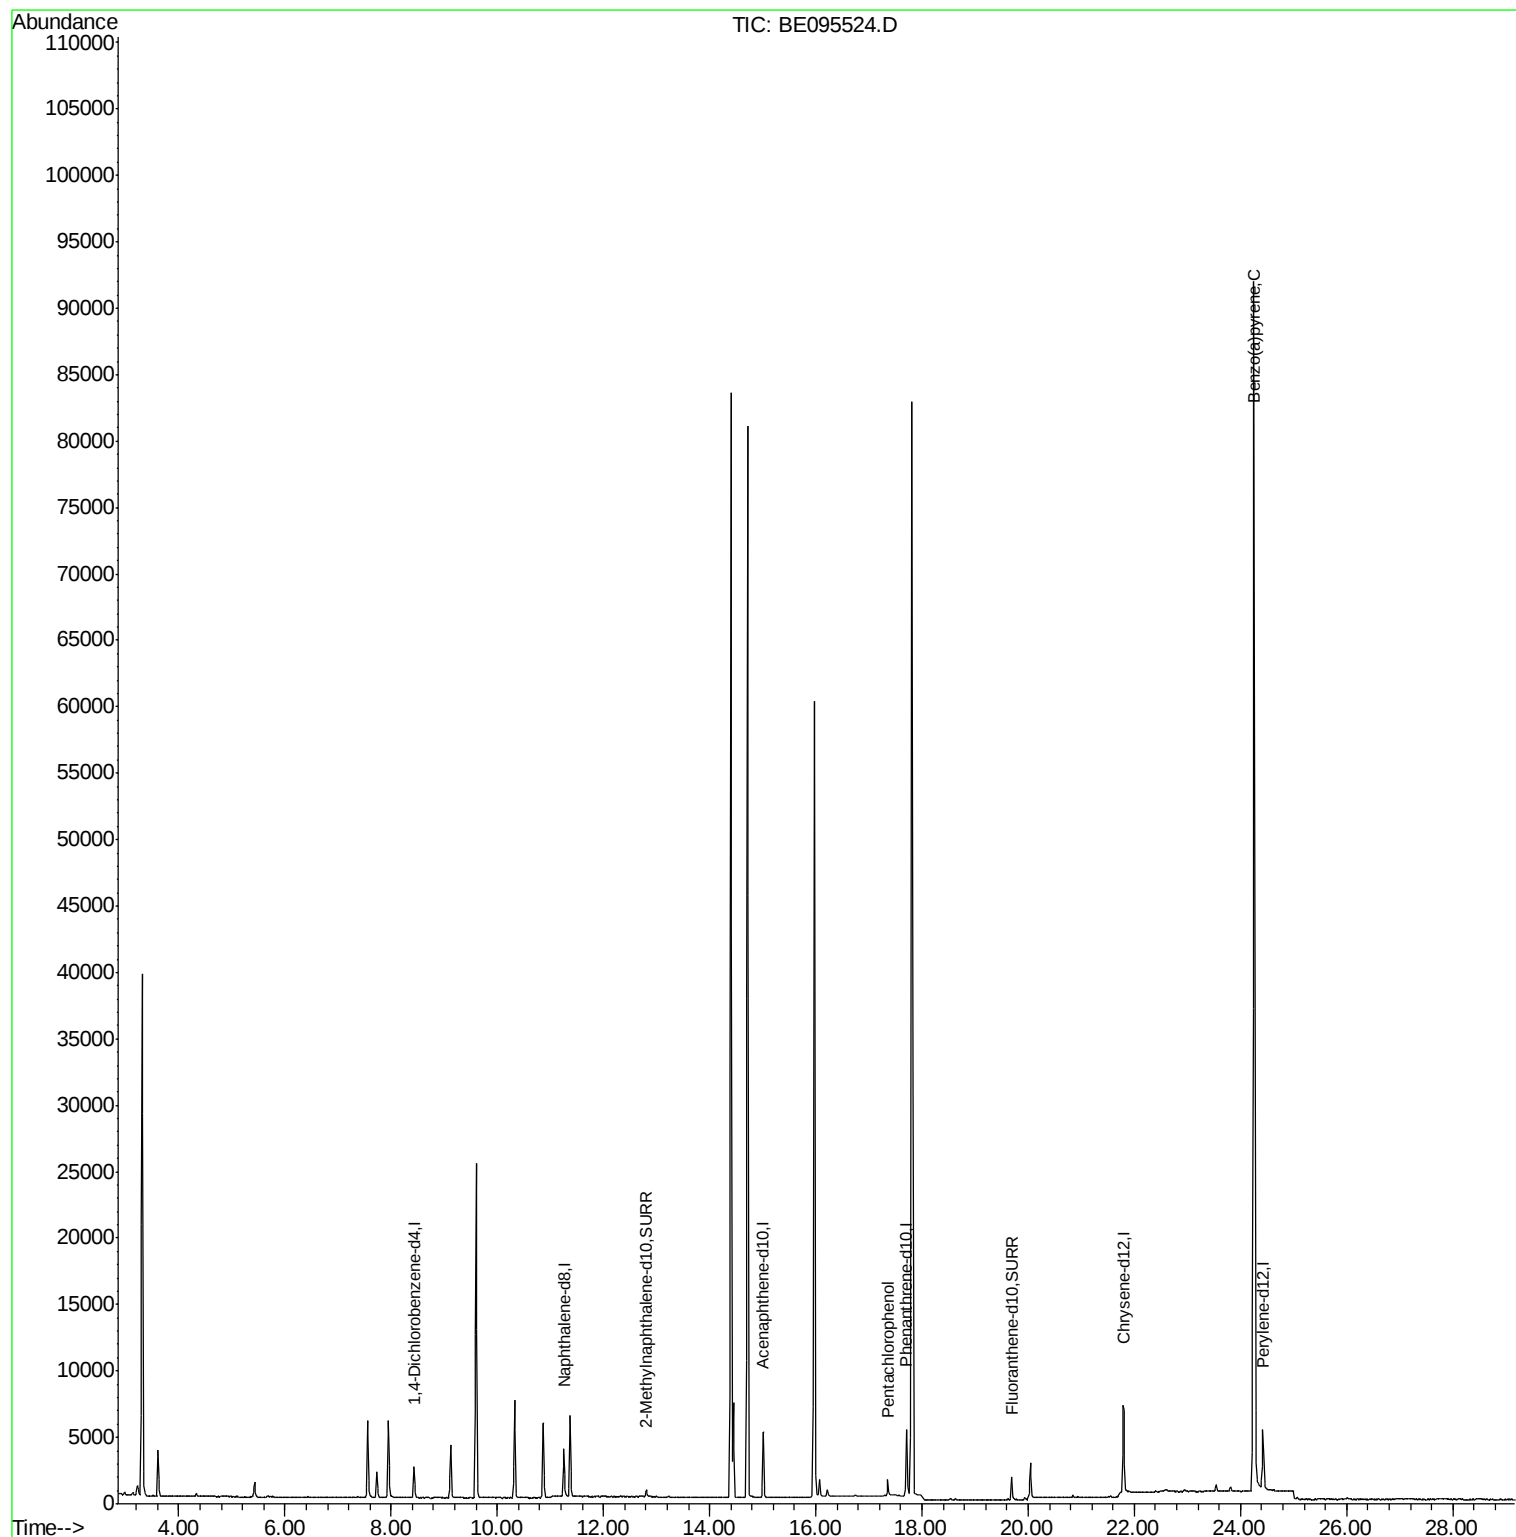


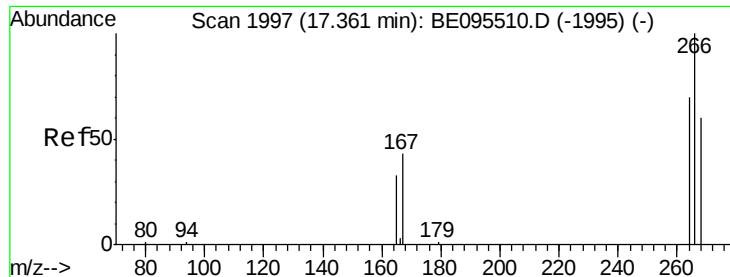

#11
 Pentachlorophenol
 Concen: 0.581 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095524.D
 Acq: 6 Feb 2018 11:02

Instrument :
 BNA_E
 ClientSampleId :
 F6C23DL

Tgt Ion: 266 Resp: 789
 Ion Ratio Lower Upper
 266 100
 264 63.2 47.9 71.9
 268 62.0 49.8 74.8

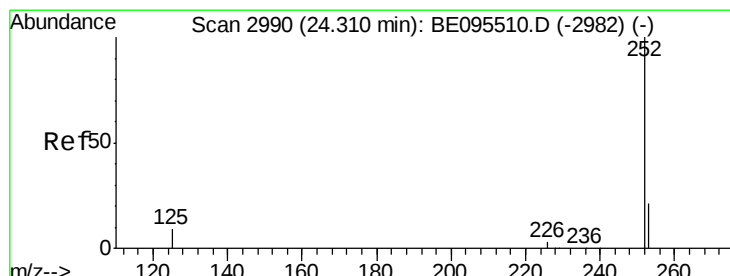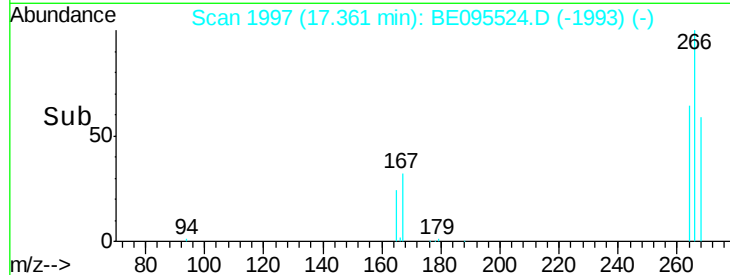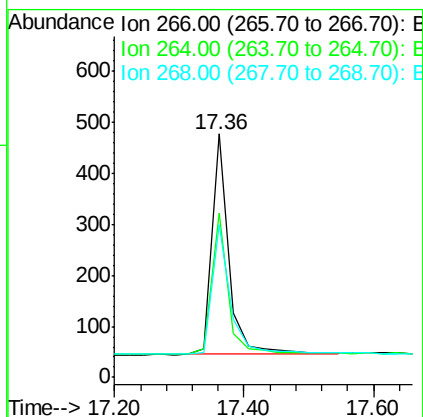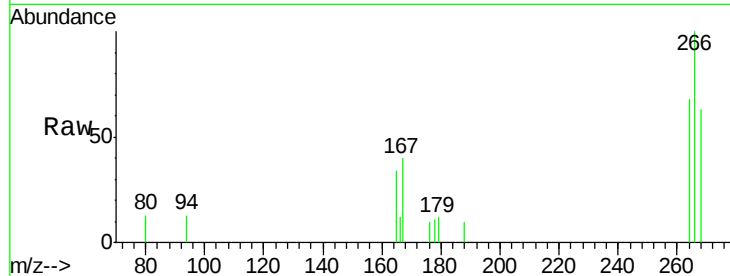

#23
 Benzo(a)pyrene
 Concen: 0.024 ng/ul
 RT: 24.26 min Scan# 2984
 Delta R.T. -0.05 min
 Lab File: BE095524.D
 Acq: 6 Feb 2018 11:02

Tgt Ion: 252 Resp: 554
 Ion Ratio Lower Upper
 252 100
 253 63.5 28.5 42.7#
 125 101.0 18.1 27.1#

