

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
 Data File : BE095525.D
 Acq On : 6 Feb 2018 11:38
 Operator : SJ/JU
 Sample : J1296-02DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C20DL

Quant Time: Feb 06 12:23:16 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 04:22:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1719	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4792	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	2901	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7187	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7007	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7124	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	666	0.09	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	1734	0.06	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.30	128	1244	0.093	ng/ul#	83
11) Pentachlorophenol	17.36	266	1511	1.085	ng/ul	99
23) Benzo(a)pyrene	24.26	252	492	0.022	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095525.D
Acq On : 6 Feb 2018 11:38
Operator : SJ/JU
Sample : J1296-02DL 5X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C20DL

Quant Time: Feb 06 12:23:16 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

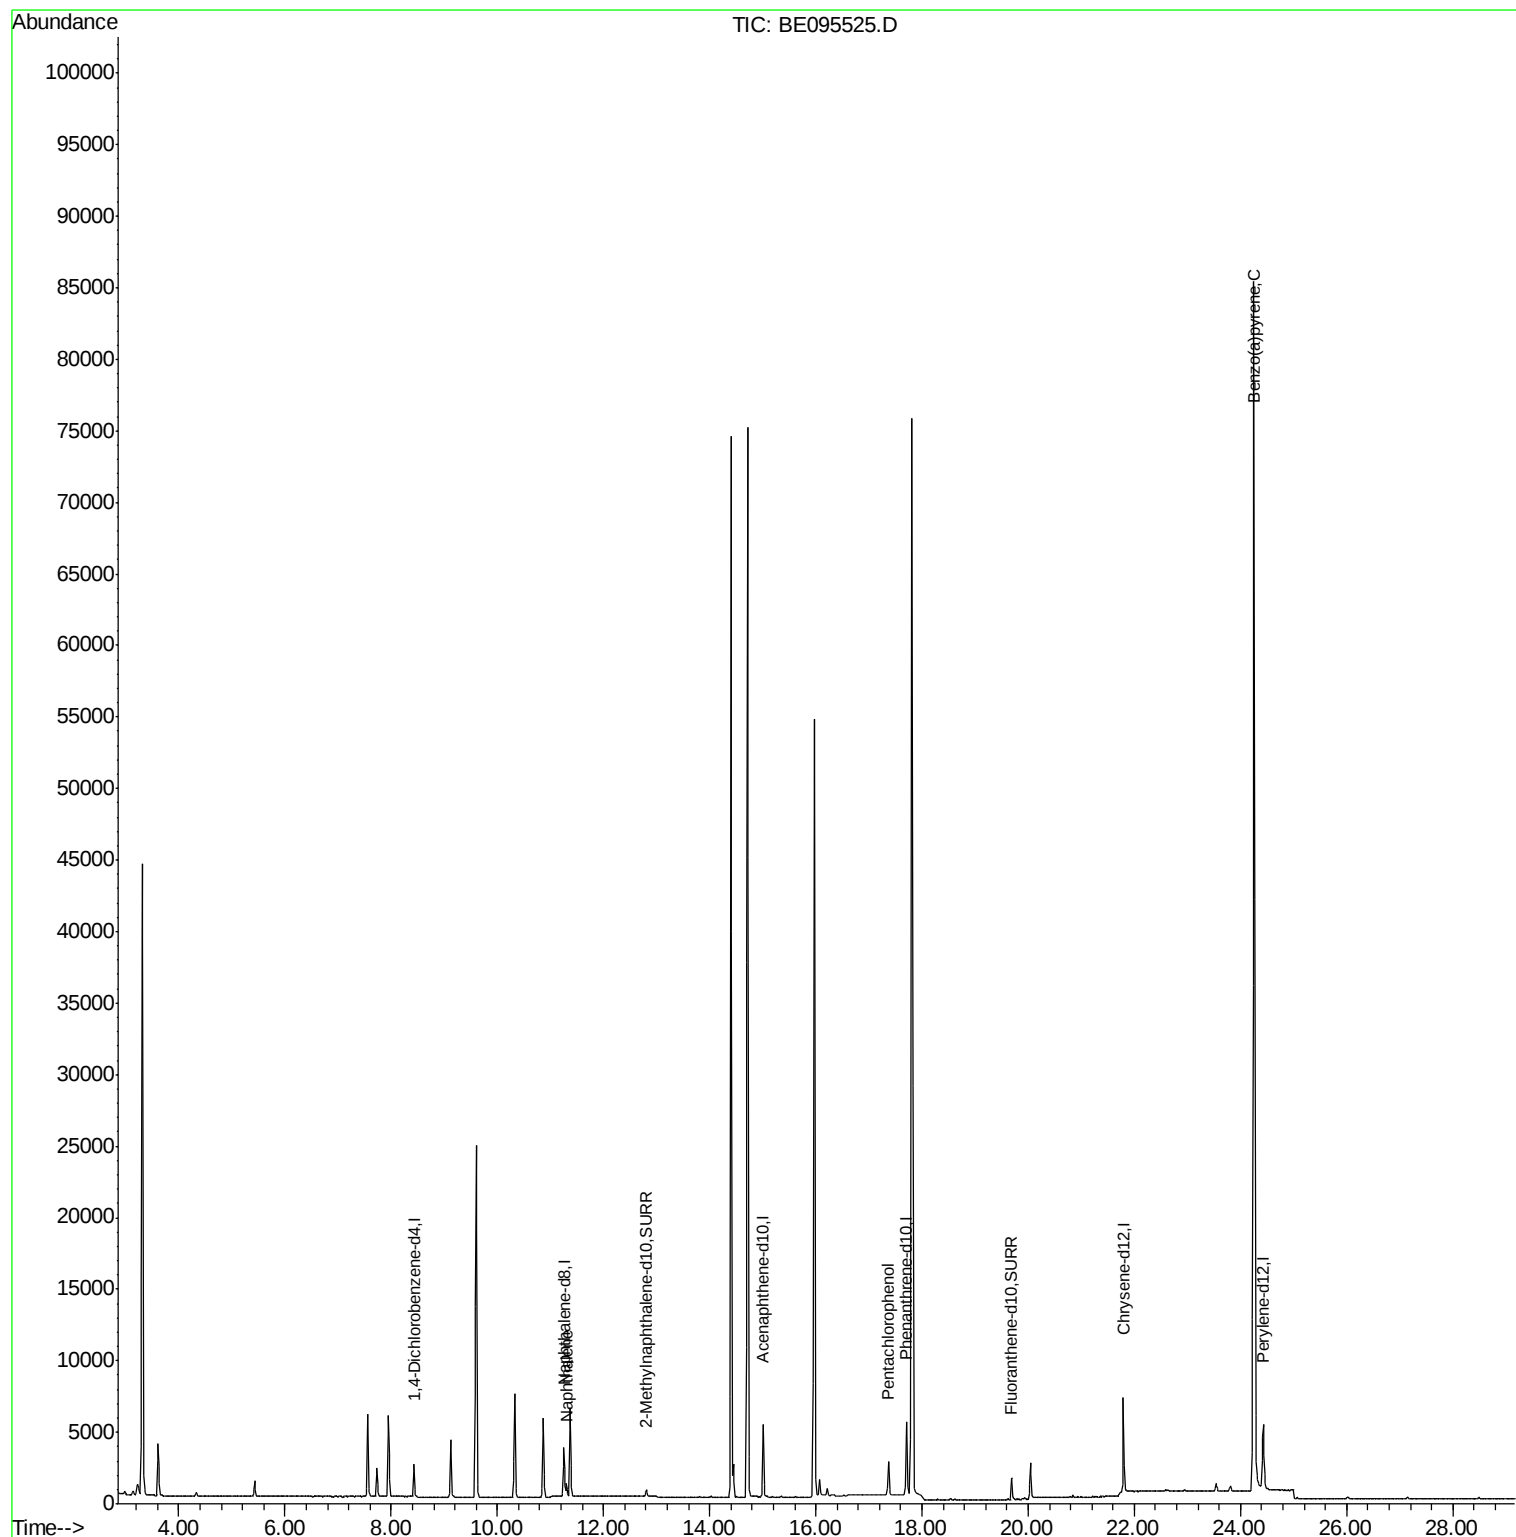

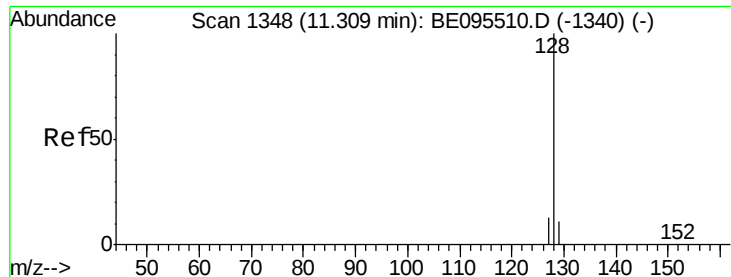

#3

Naphthalene

Concen: 0.093 ng/ul

RT: 11.30 min Scan# 1347

Delta R.T. -0.01 min

Lab File: BE095525.D

Acq: 6 Feb 2018 11:38

Instrument :

BNA_E

ClientSampleId :

F6C20DL


Tgt Ion:128 Resp: 1244

Ion Ratio Lower Upper

128 100

129 17.1 11.3 16.9#




127 19.8 4.0 6.0#

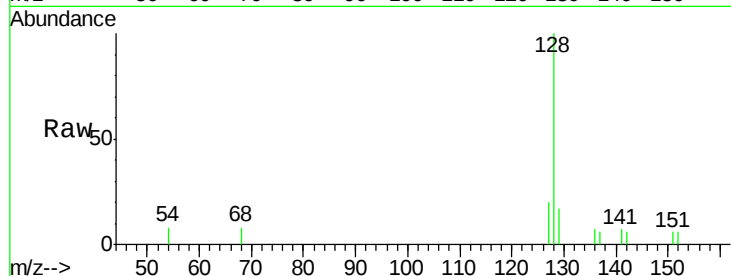

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

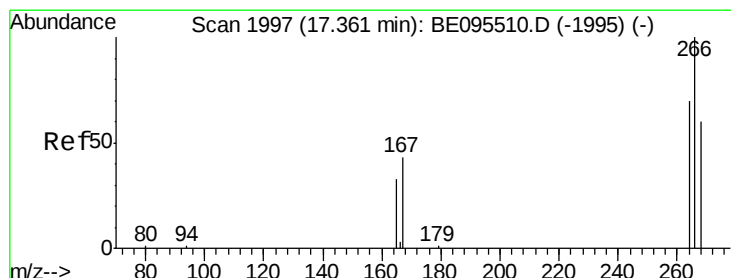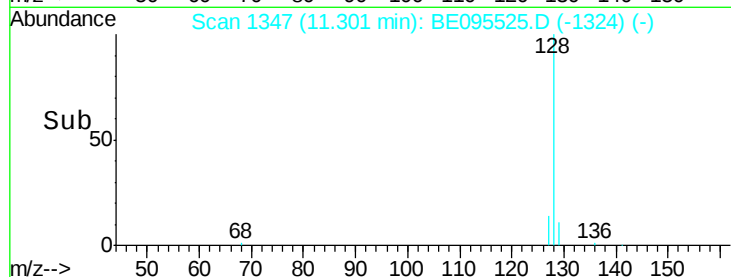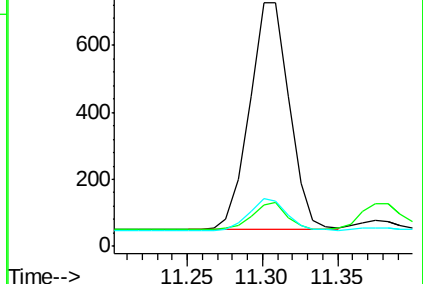

#11

Pentachlorophenol

Concen: 1.085 ng/ul

RT: 17.36 min Scan# 1997

Delta R.T. 0.00 min

Lab File: BE095525.D

Acq: 6 Feb 2018 11:38


Tgt Ion:266 Resp: 1511

Ion Ratio Lower Upper

266 100

264 61.4 47.9 71.9



268 63.1 49.8 74.8

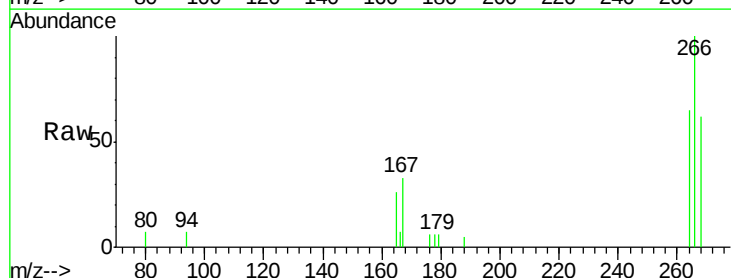


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

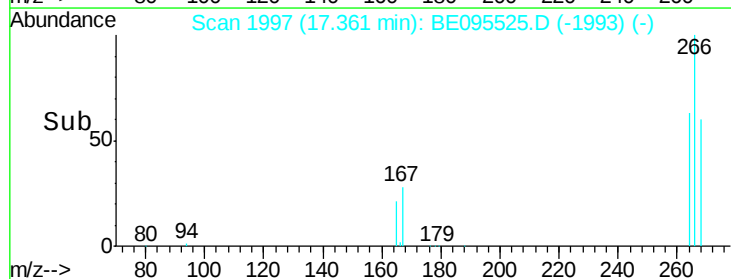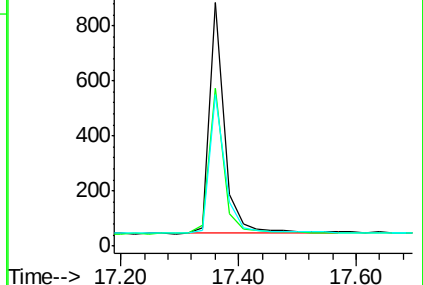

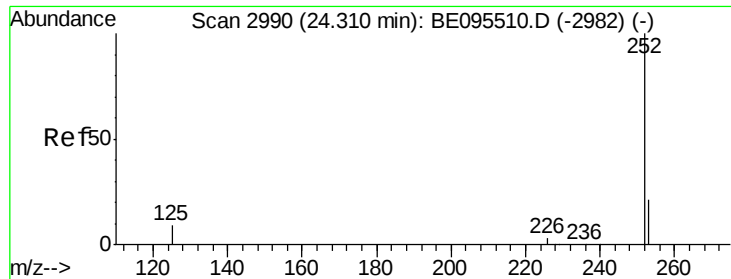

#23

Benzo(a)pyrene

Concen: 0.022 ng/ul

RT: 24.26 min Scan# 2984

Delta R.T. -0.05 min

Lab File: BE095525.D


Acq: 6 Feb 2018 11:38

Instrument :

BNA_E

ClientSampleId :

F6C20DL

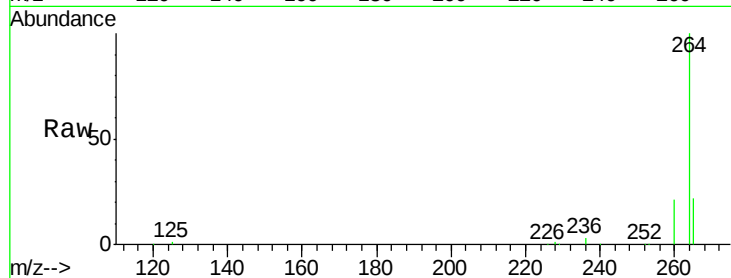

Tgt Ion: 252 Resp: 492

Ion Ratio Lower Upper

252 100

253 69.4 28.5 42.7#

125 108.2 18.1 27.1#

