

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
 Data File : BE095526.D
 Acq On : 6 Feb 2018 12:14
 Operator : SJ/JU
 Sample : J1296-03DL 5X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C21DL

Quant Time: Feb 06 13:20:42 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 04:22:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1753	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4956	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3003	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7401	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7185	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7454	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	567	0.07	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	1500	0.05	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.30	128	880	0.063	ng/ul#	80
11) Pentachlorophenol	17.36	266	1651	1.152	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095526.D
Acq On : 6 Feb 2018 12:14
Operator : SJ/JU
Sample : J1296-03DL 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C21DL

Quant Time: Feb 06 13:20:42 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

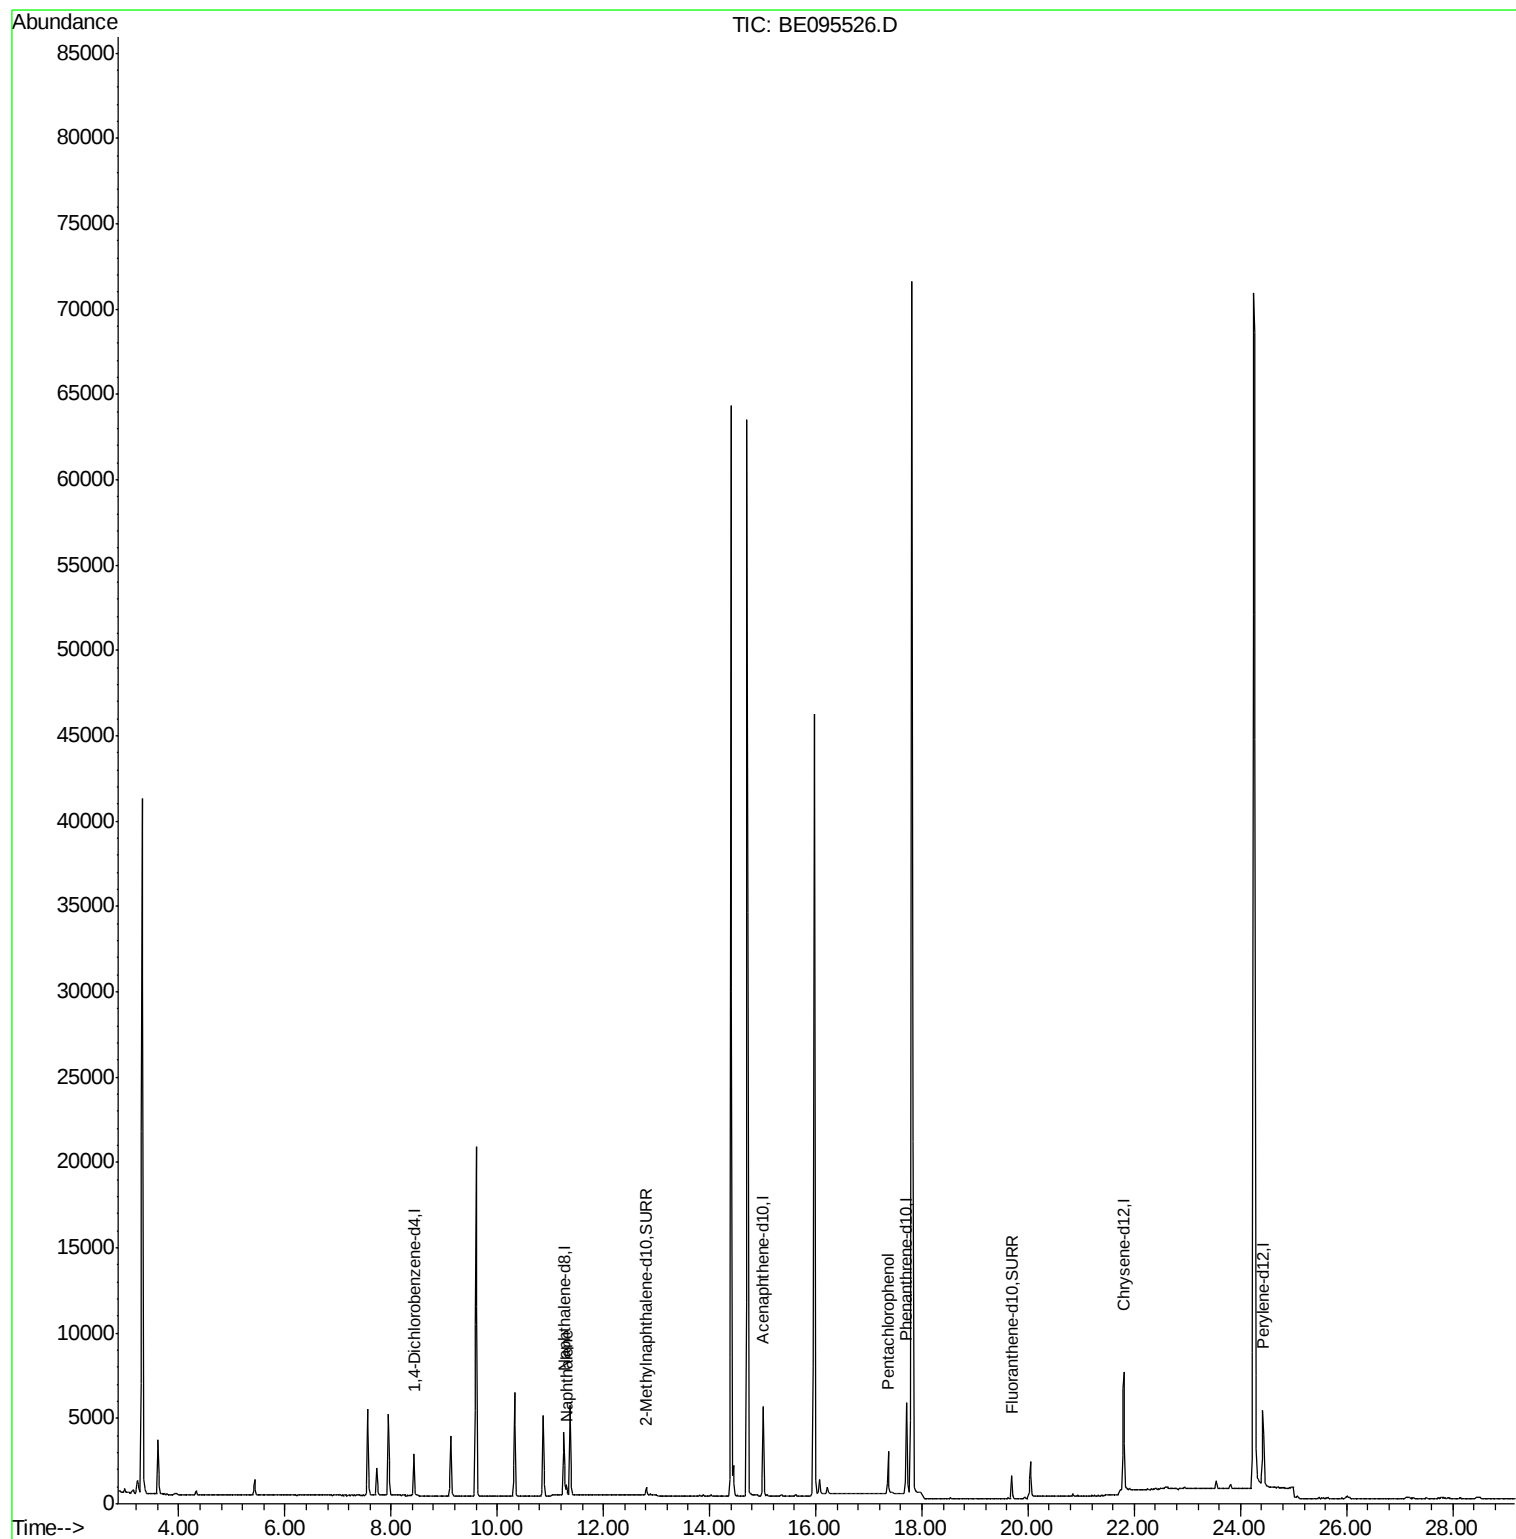

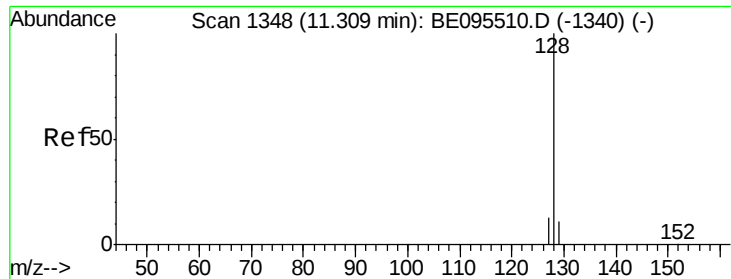

#3

Naphthalene

Concen: 0.063 ng/ul

RT: 11.30 min Scan# 1347

Delta R.T. -0.01 min

Lab File: BE095526.D

Acq: 6 Feb 2018 12:14

Instrument :

BNA_E

ClientSampleId :

F6C21DL


Tgt Ion:128 Resp: 880

Ion Ratio Lower Upper

128 100

129 18.2 11.3 16.9#


127 20.9 4.0 6.0#

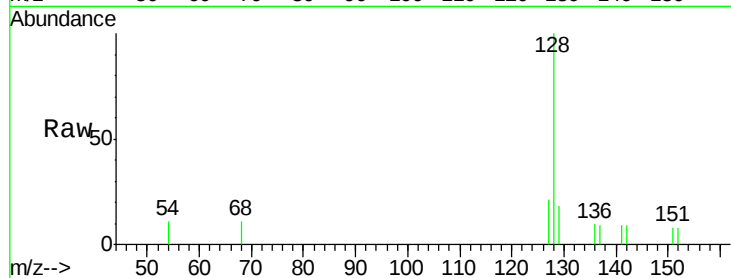



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

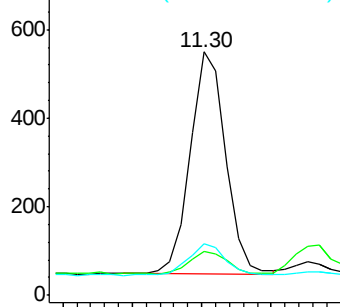

Time--> 11.20 11.25 11.30 11.35

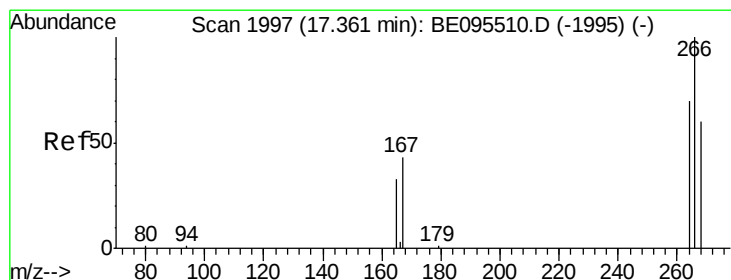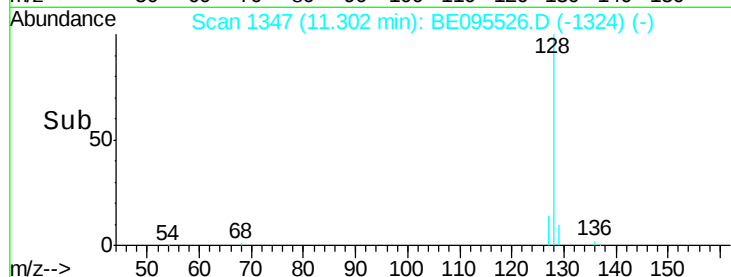

#11

Pentachlorophenol

Concen: 1.152 ng/ul

RT: 17.36 min Scan# 1997

Delta R.T. 0.00 min

Lab File: BE095526.D

Acq: 6 Feb 2018 12:14


Tgt Ion:266 Resp: 1651

Ion Ratio Lower Upper

266 100

264 60.6 47.9 71.9


268 62.9 49.8 74.8

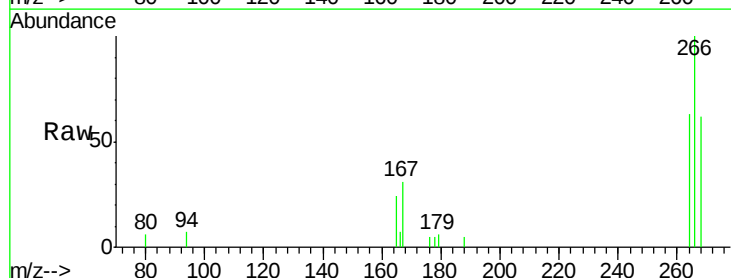

Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

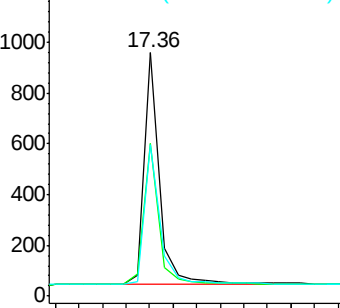

Time--> 17.20 17.40 17.60

