


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095491.D
Acq On : 5 Feb 2018 15:23
Operator : SJ/JU
Sample : J1315-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C63

Manual Integrations
APPROVED

Sohil
2/6/2018 2:30:42 PM

Quant Time: Feb 06 01:52:24 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 01:31:24 2018
Response via : Initial Calibration

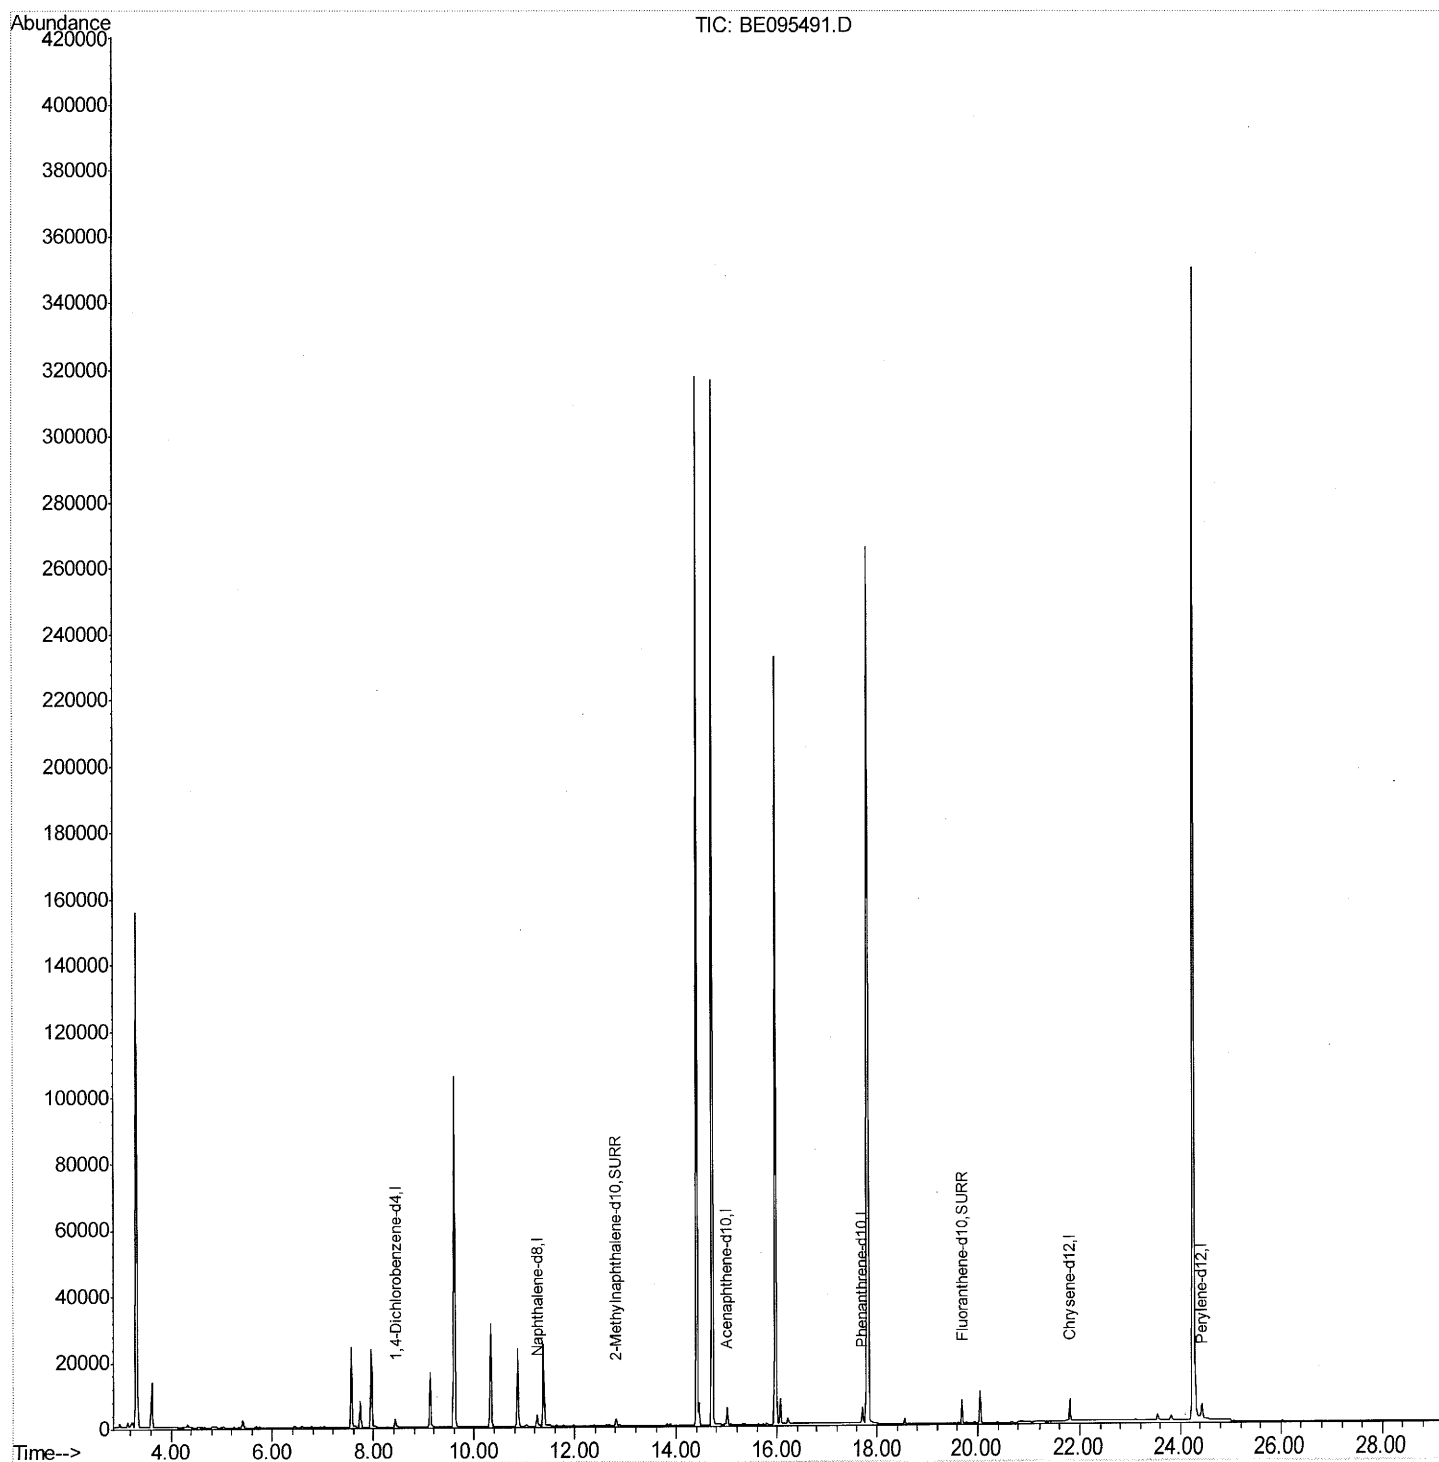

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095491.D
 Acq On : 5 Feb 2018 15:23
 Operator : SJ/JU
 Sample : J1315-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6C63

Manual Integrations
 APPROVED

Sohil
 2/6/2018 2:30:42 PM

Quant Time: Feb 06 01:32:13 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 01:31:24 2018
 Response via : Initial Calibration

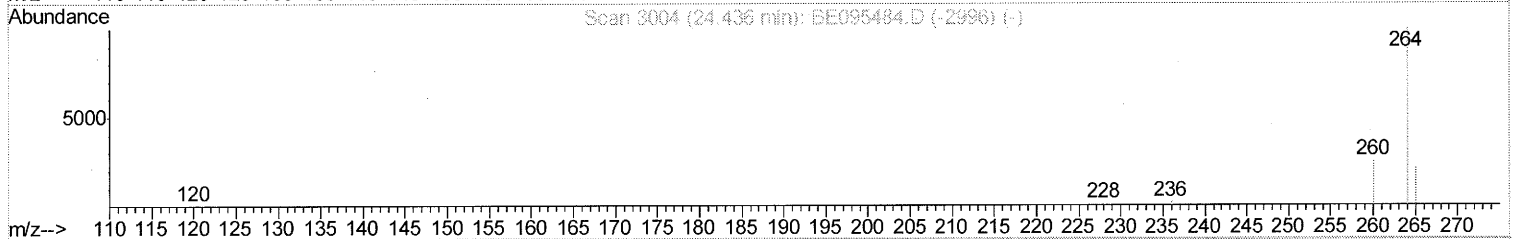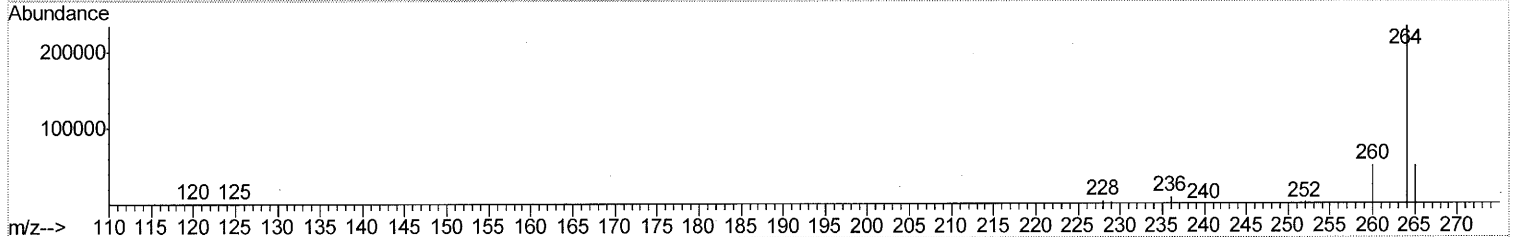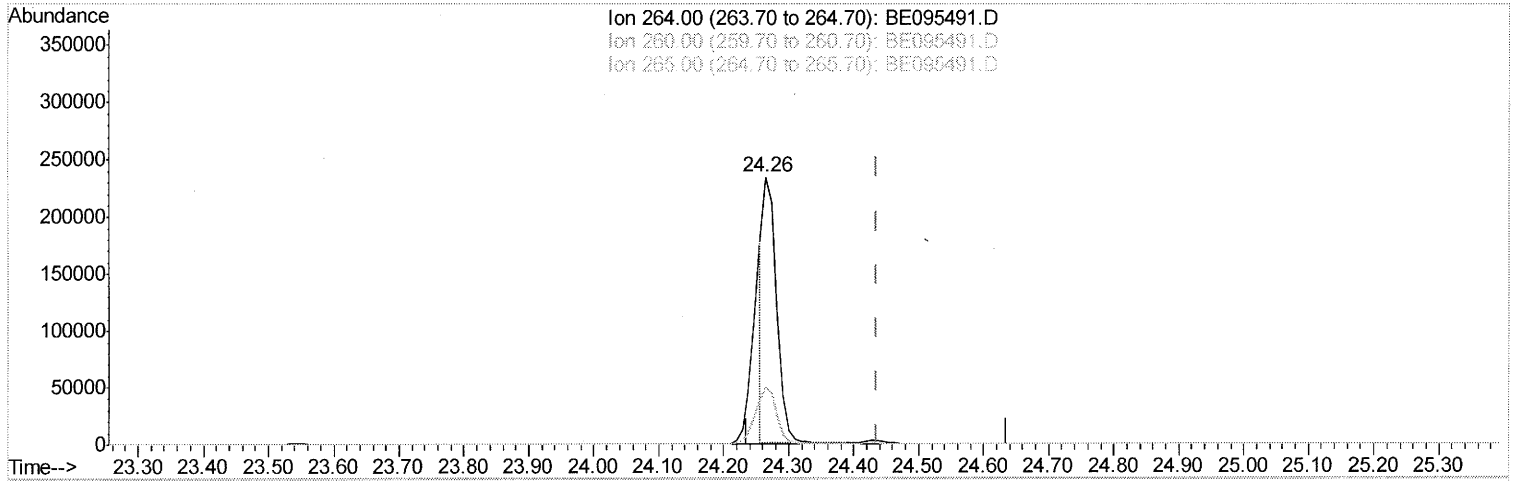

TIC: BE095491.D

(20) Perylene-d12 (I)

24.264min (-0.172) 0.40ng/ul

response 338732

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.42#
265.00	103.50	21.35#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095491.D
 Acq On : 5 Feb 2018 15:23
 Operator : SJ/JU
 Sample : J1315-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6C63

Manual Integrations
 APPROVED

Sohil
 2/6/2018 2:30:42 PM

Quant Time: Feb 06 01:32:13 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 01:31:24 2018
 Response via : Initial Calibration

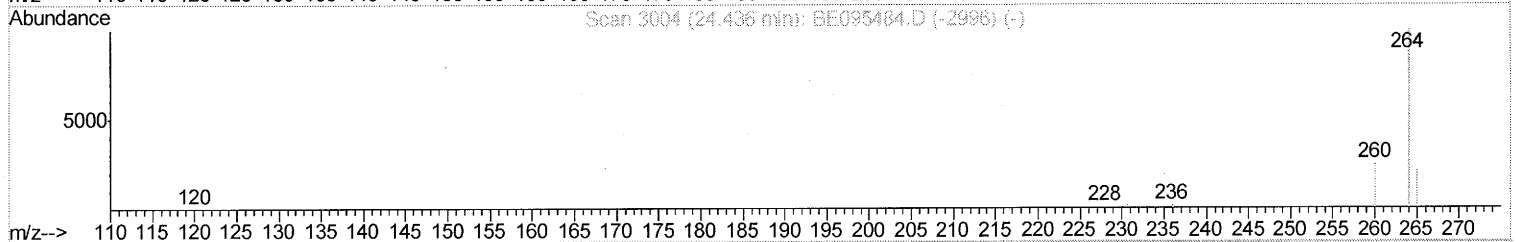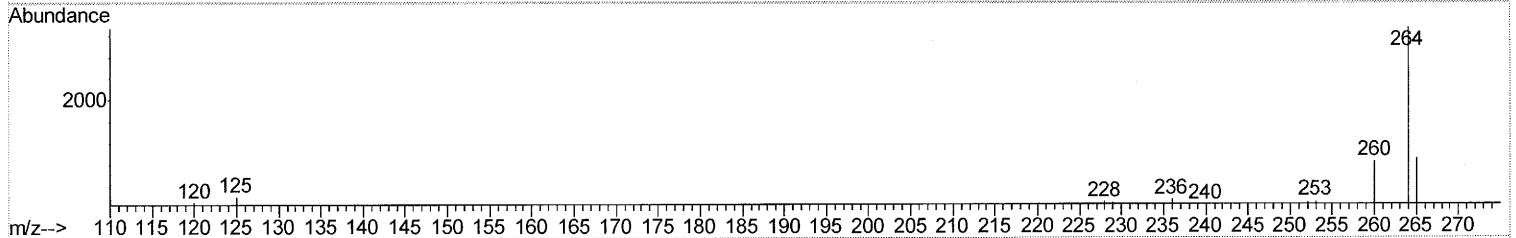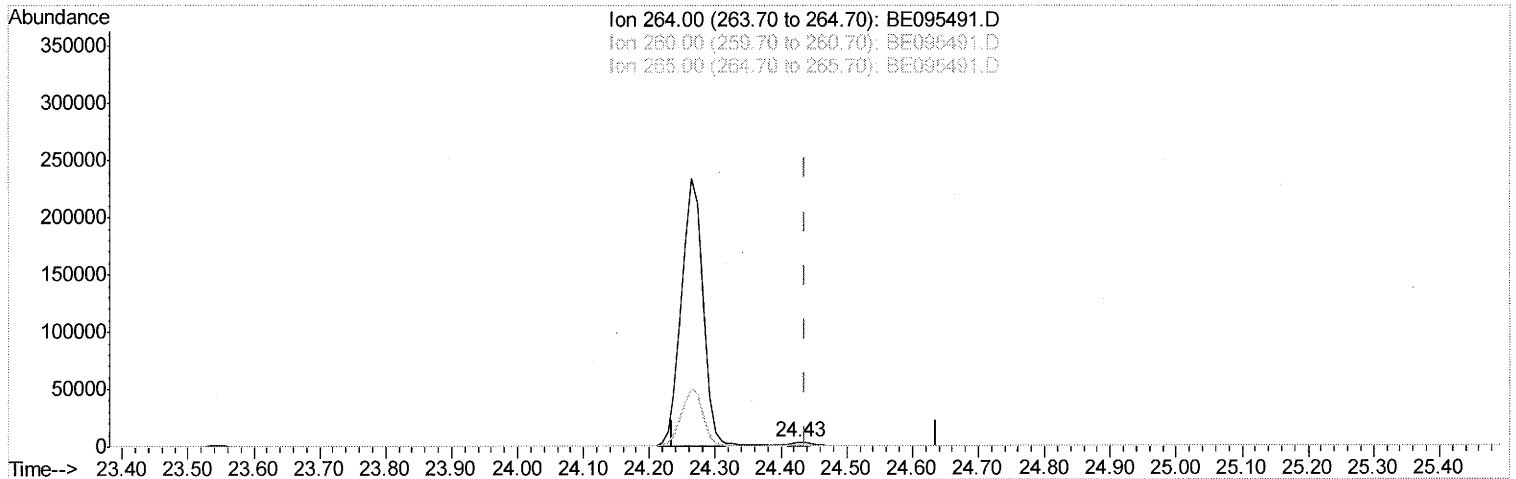

TIC: BE095491.D

(20) Perylene-d12 (I)

24.427min (-0.010) 0.40ng/ul m

response 6333

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.50
265.00	103.50	26.91#
0.00	0.00	0.00

SJ 2/7/18

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095491.D
Acq On : 5 Feb 2018 15:23
Operator : SJ/JU
Sample : J1315-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C63

Manual Integrations
APPROVED

Sohil
2/6/2018 2:30:42 PM

Quant Time: Feb 06 01:52:24 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 01:31:24 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1787	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	4947	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3140	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7094	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6989	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	6333m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	2666	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7722	0.28	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ 2/7/18