


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095505.D
Acq On : 5 Feb 2018 23:45
Operator : SJ/JU
Sample : J1314-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C39

Manual Integrations
APPROVED

Sohil
2/6/2018 2:31:22 PM

Quant Time: Feb 06 03:30:14 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration

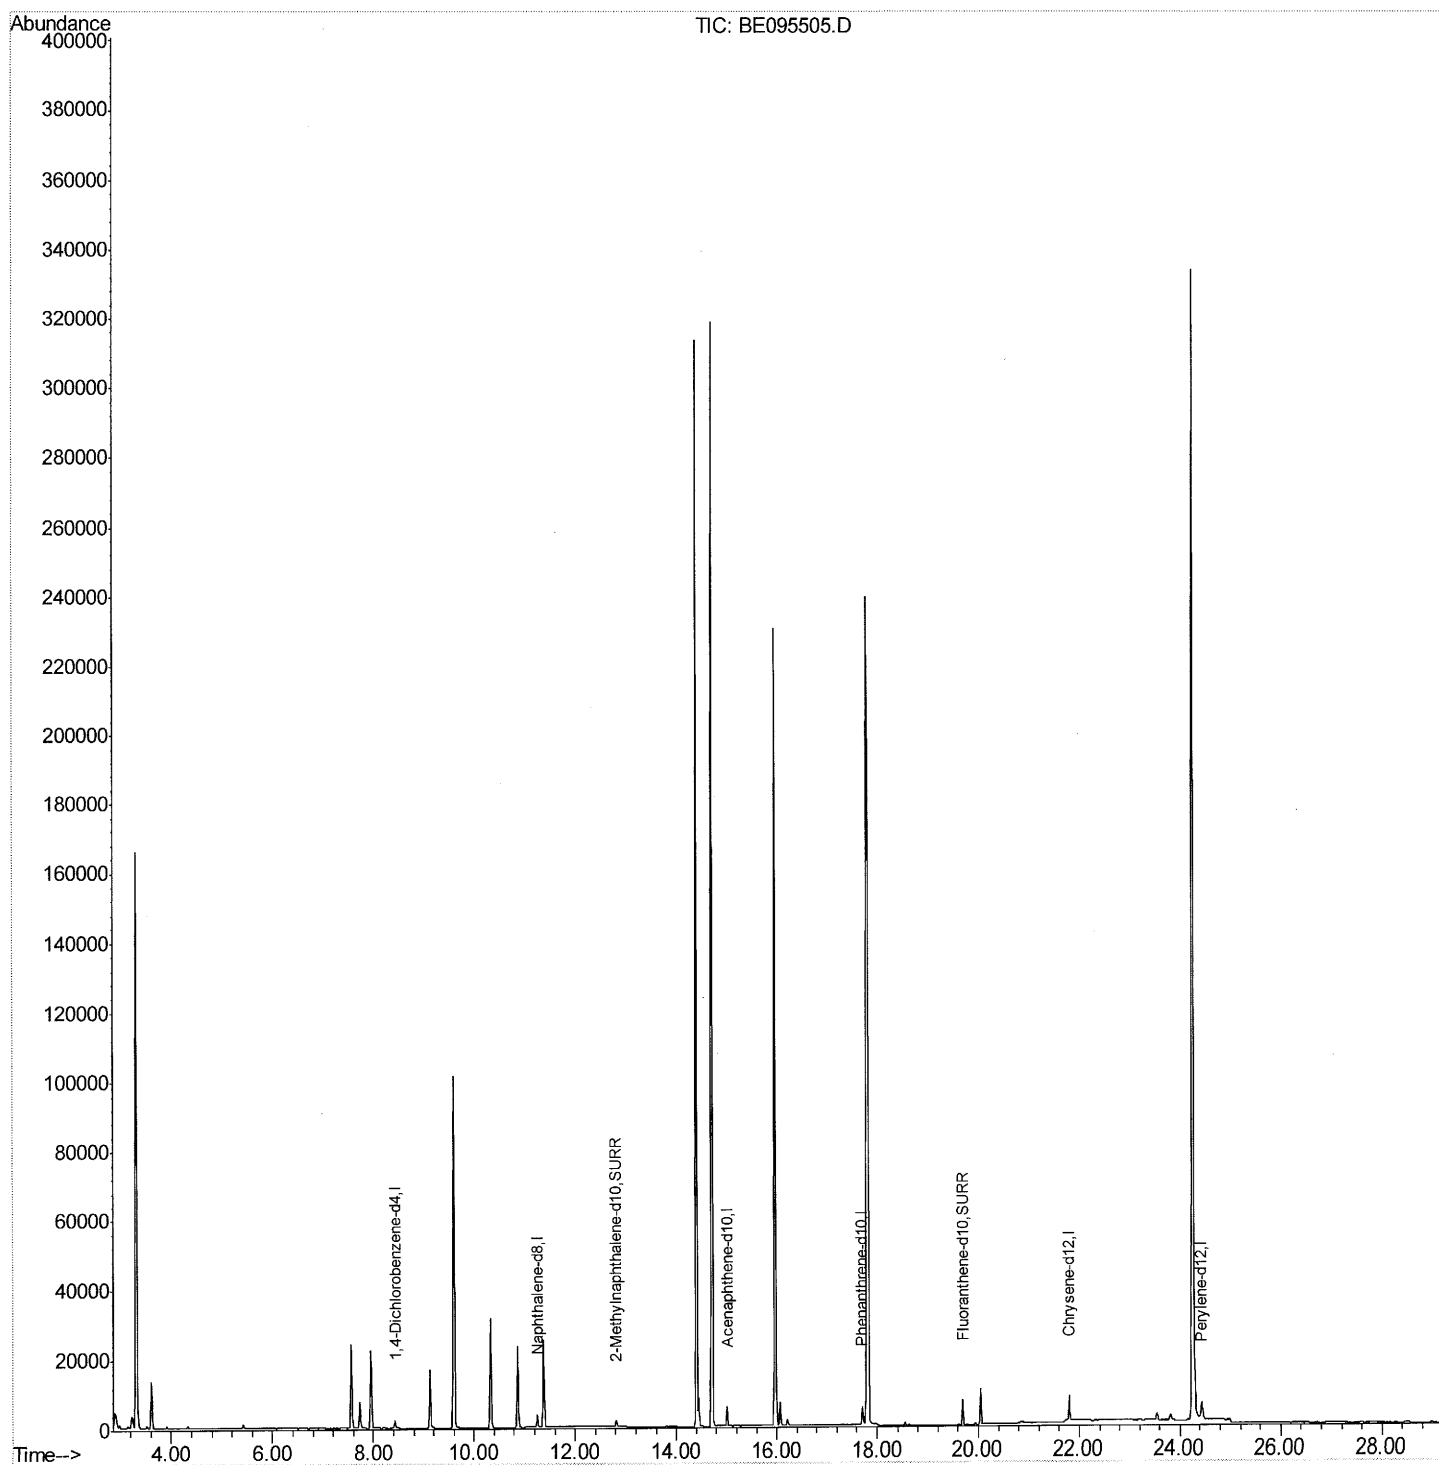

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095505.D
Acq On : 5 Feb 2018 23:45
Operator : SJ/JU
Sample : J1314-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6C39

Manual Integrations
APPROVED

Sohil
2/6/2018 2:31:22 PM

Quant Time: Feb 06 02:11:25 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration

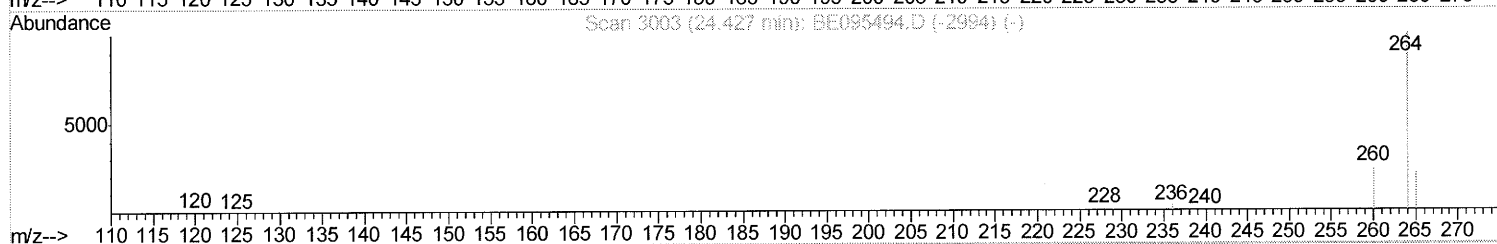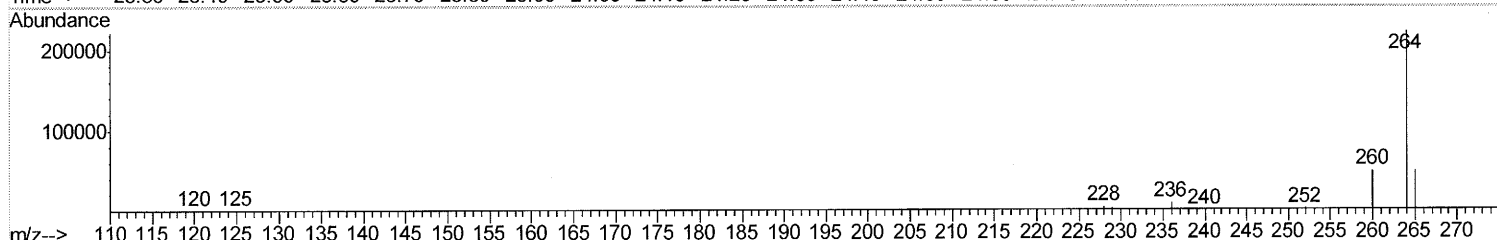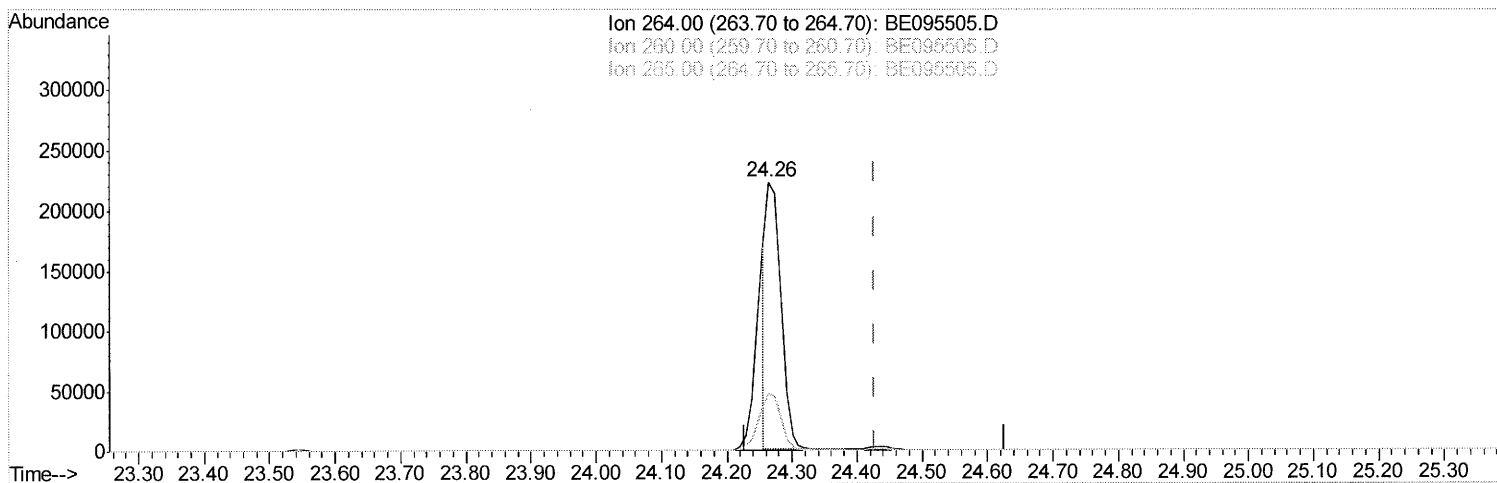

TIC: BE095505.D

(20) Perylene-d12 (I)

24.265min (-0.163) 0.40ng/ul

response 341262

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.37#
265.00	103.50	21.22#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095505.D
Acq On : 5 Feb 2018 23:45
Operator : SJ/JU
Sample : J1314-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C39

Manual Integrations
APPROVED

Sohil
2/6/2018 2:31:22 PM

Quant Time: Feb 06 02:11:25 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration

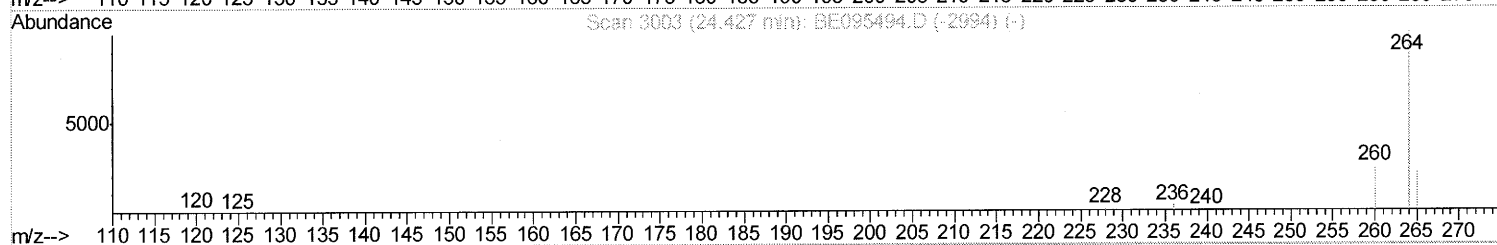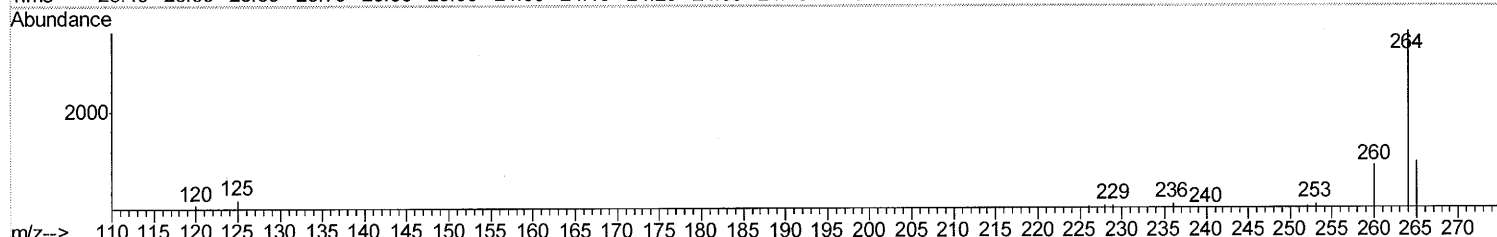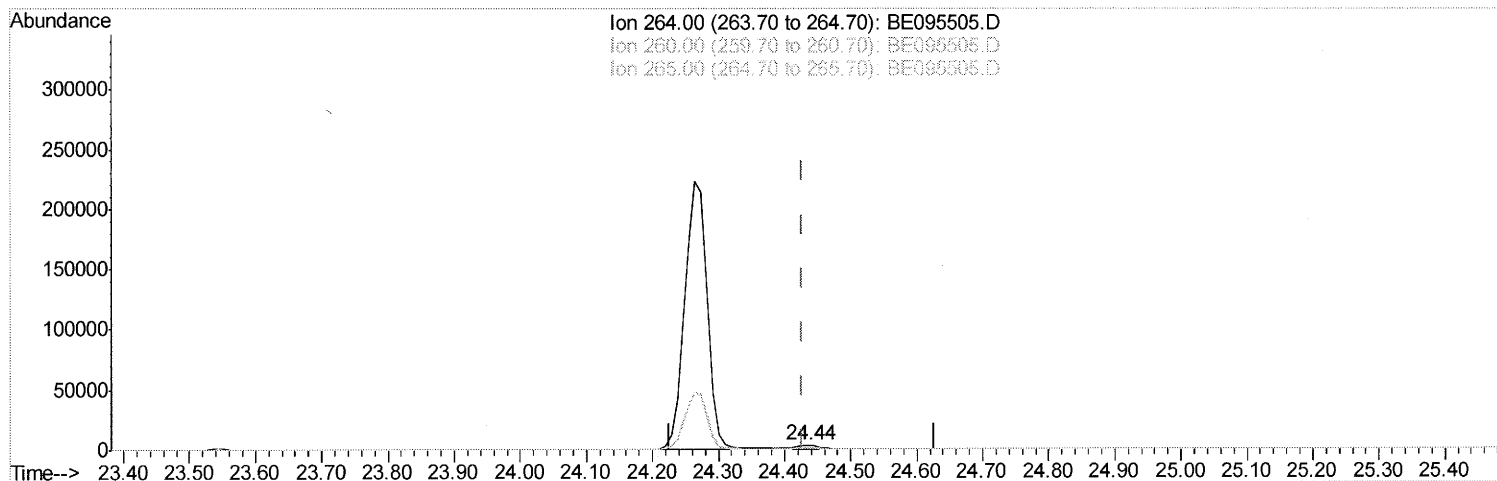

TIC: BE095505.D

(20) Perylene-d12 (I)

24.436min (+0.009) 0.40ng/ul m

response 7140

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.60
265.00	103.50	27.89#
0.00	0.00	0.00

35 2/7/18

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095505.D
Acq On : 5 Feb 2018 23:45
Operator : SJ/JU
Sample : J1314-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C39

Manual Integrations
APPROVED

Sohil
2/6/2018 2:31:22 PM

Quant Time: Feb 06 03:30:14 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1859	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5207	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3319	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7671	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7581	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	7140m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	2588	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7828	0.27	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ 2/7/18