


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095507.D
Acq On : 6 Feb 2018 00:56
Operator : SJ/JU
Sample : J1314-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6C55

Manual Integrations
APPROVED

Sohil
2/6/2018 2:31:28 PM

Quant Time: Feb 06 03:34:47 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration

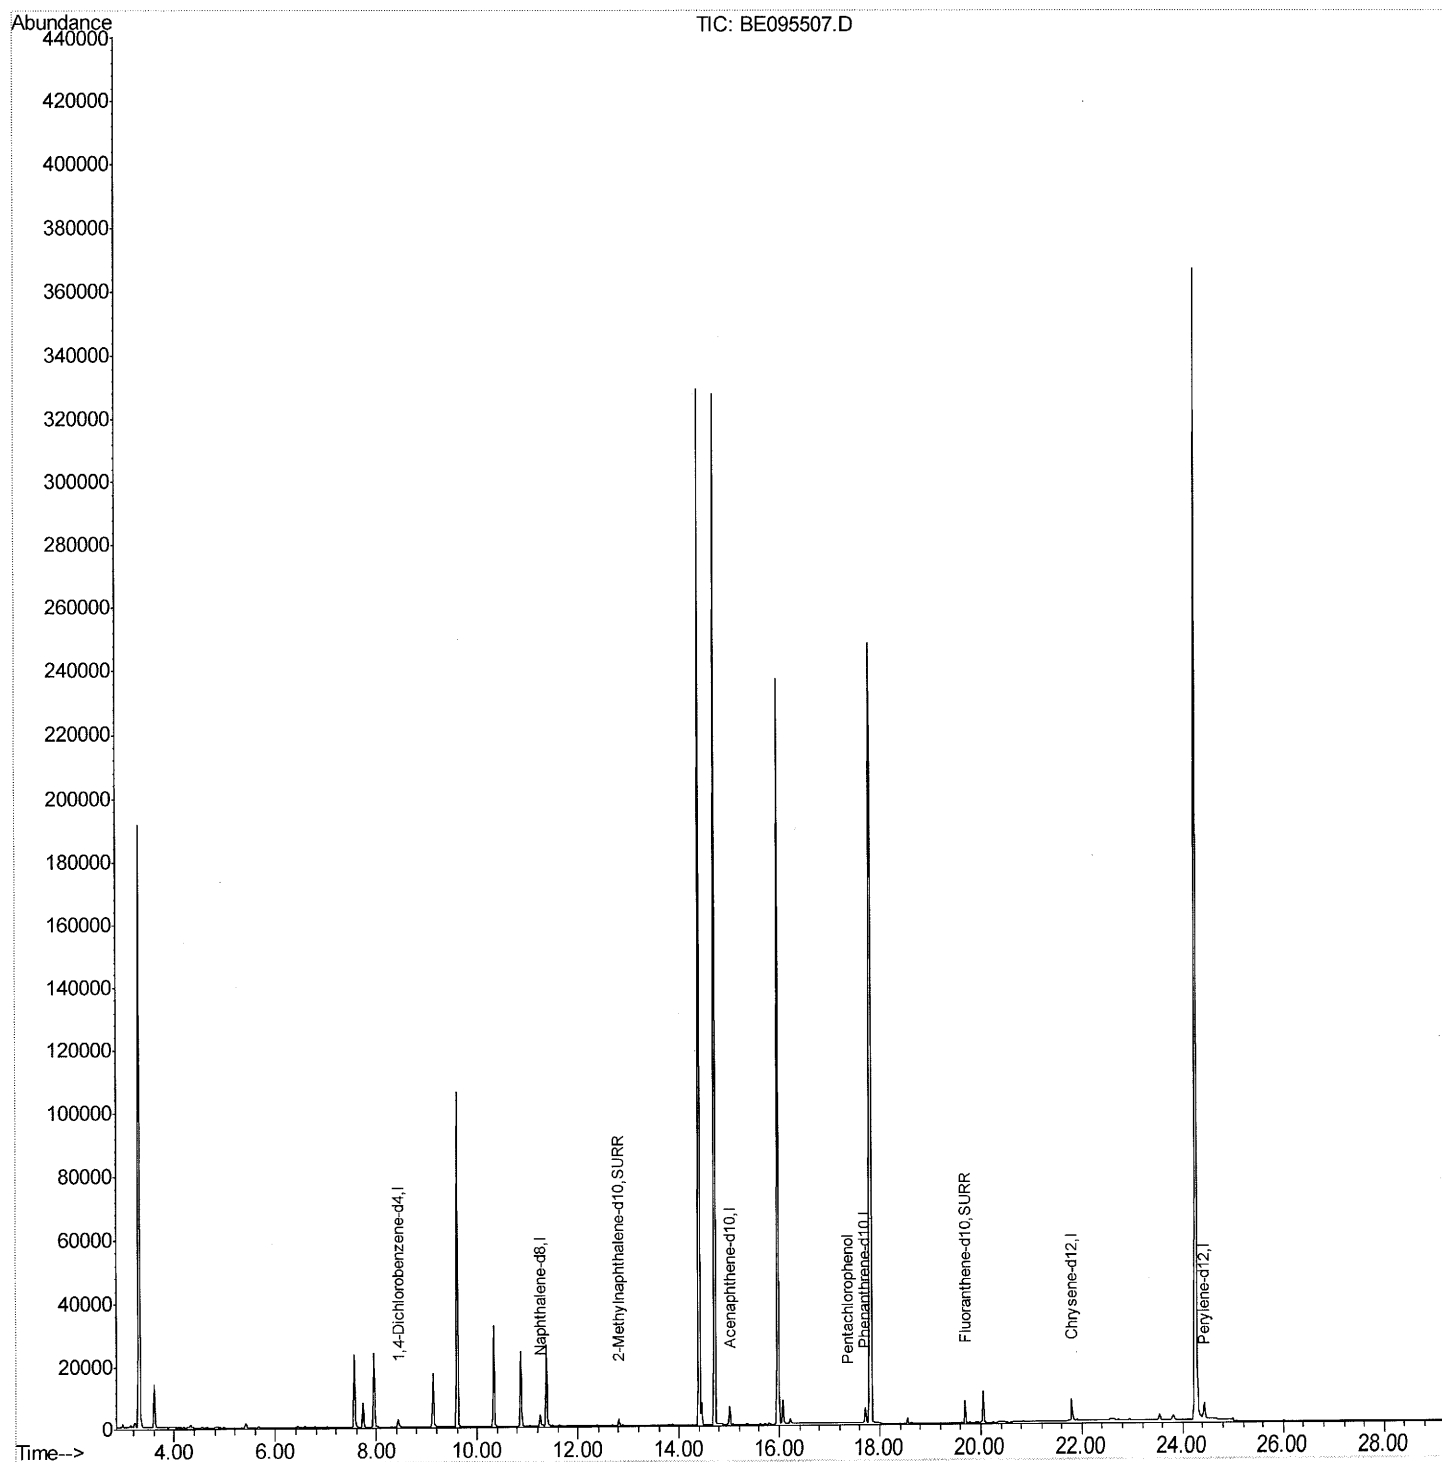

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095507.D
Acq On : 6 Feb 2018 00:56
Operator : SJ/JU
Sample : J1314-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6C55

Manual Integrations
APPROVED

Sohil
2/6/2018 2:31:28 PM

Quant Time: Feb 06 02:11:39 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration

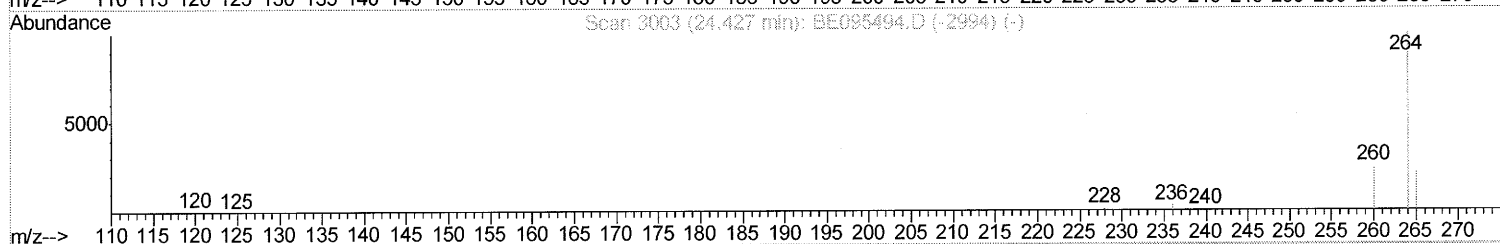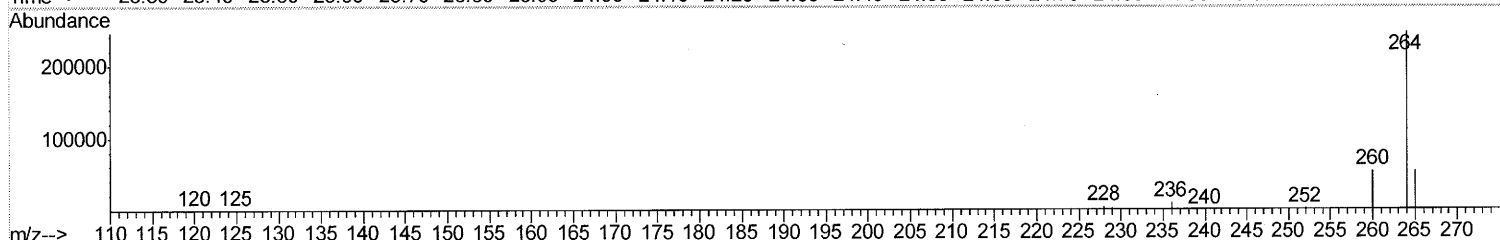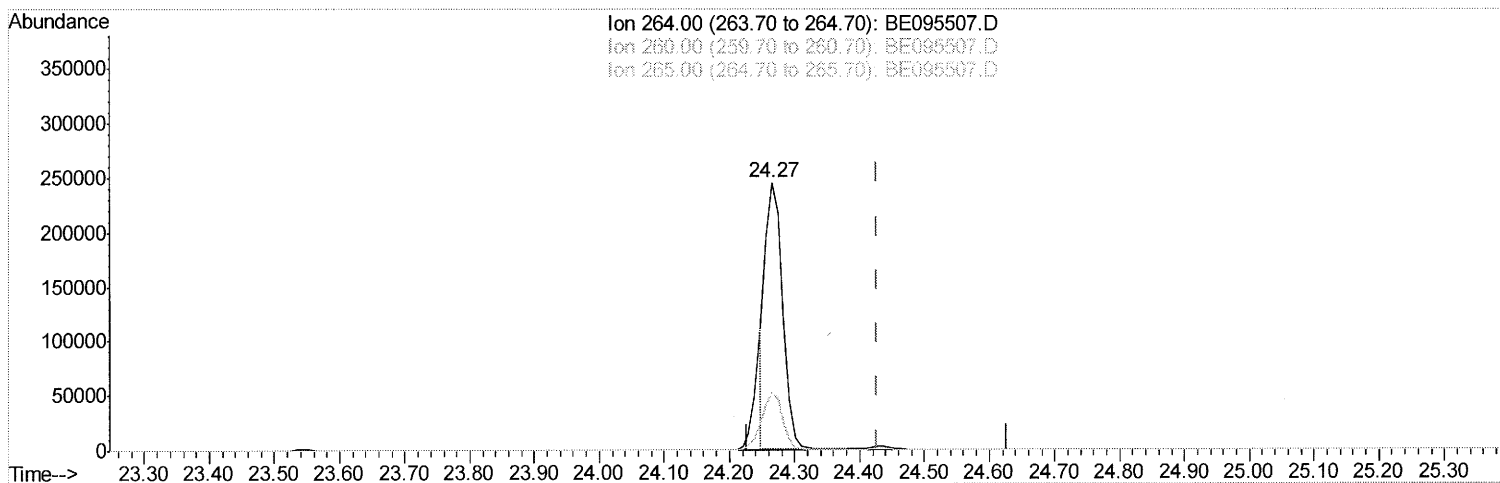

TIC: BE095507.D

(20) Perylene-d12 (I)

24.265min (-0.162) 0.40ng/ul

response 455081

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.31#
265.00	103.50	21.42#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095507.D
 Acq On : 6 Feb 2018 00:56
 Operator : SJ/JU
 Sample : J1314-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6C55

Manual Integrations
 APPROVED

Sohil
 2/6/2018 2:31:28 PM

Quant Time: Feb 06 02:11:39 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 02:09:13 2018
 Response via : Initial Calibration

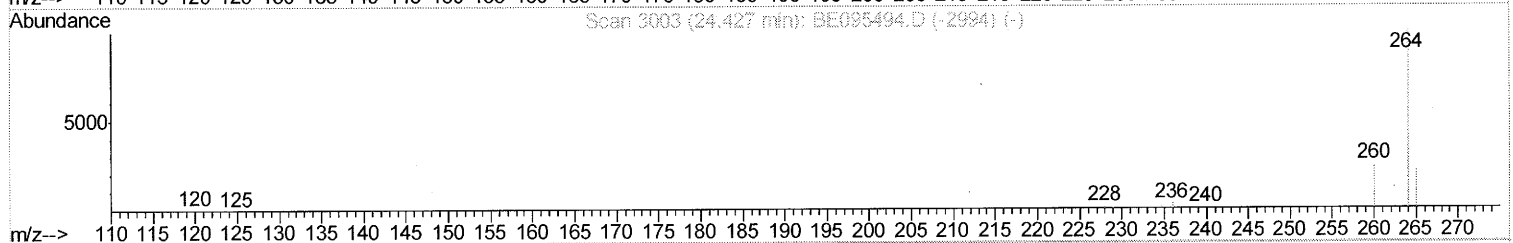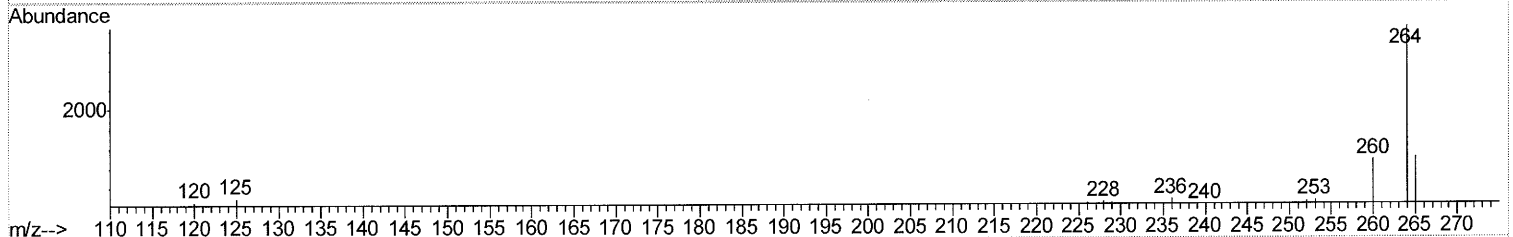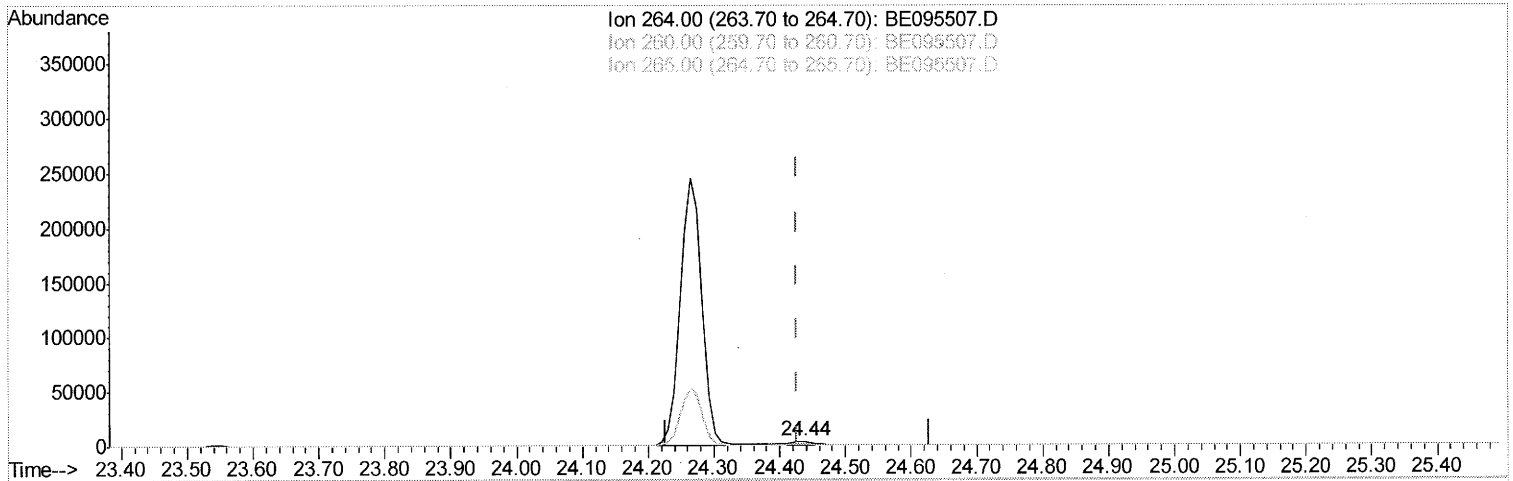

TIC: BE095507.D

(20) Perylene-d12 (I)

24.436min (+0.009) 0.40ng/ul m

SJ 2/7/18

response 7220

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.64
265.00	103.50	27.20#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095507.D
Acq On : 6 Feb 2018 00:56
Operator : SJ/JU
Sample : J1314-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6C55

Manual Integrations
APPROVED

Sohil
2/6/2018 2:31:28 PM

Quant Time: Feb 06 03:34:47 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1802	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5165	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3390	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7464	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7764	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	7220m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2717	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8197	0.29	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	130	0.090	ng/ul#	Ovalue 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed