


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095513.D
Acq On : 6 Feb 2018 4:31
Operator : SJ/JU
Sample : J1315-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C59

Manual Integrations
APPROVED

Sohil
2/6/2018 2:31:42 PM

Quant Time: Feb 06 06:24:06 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

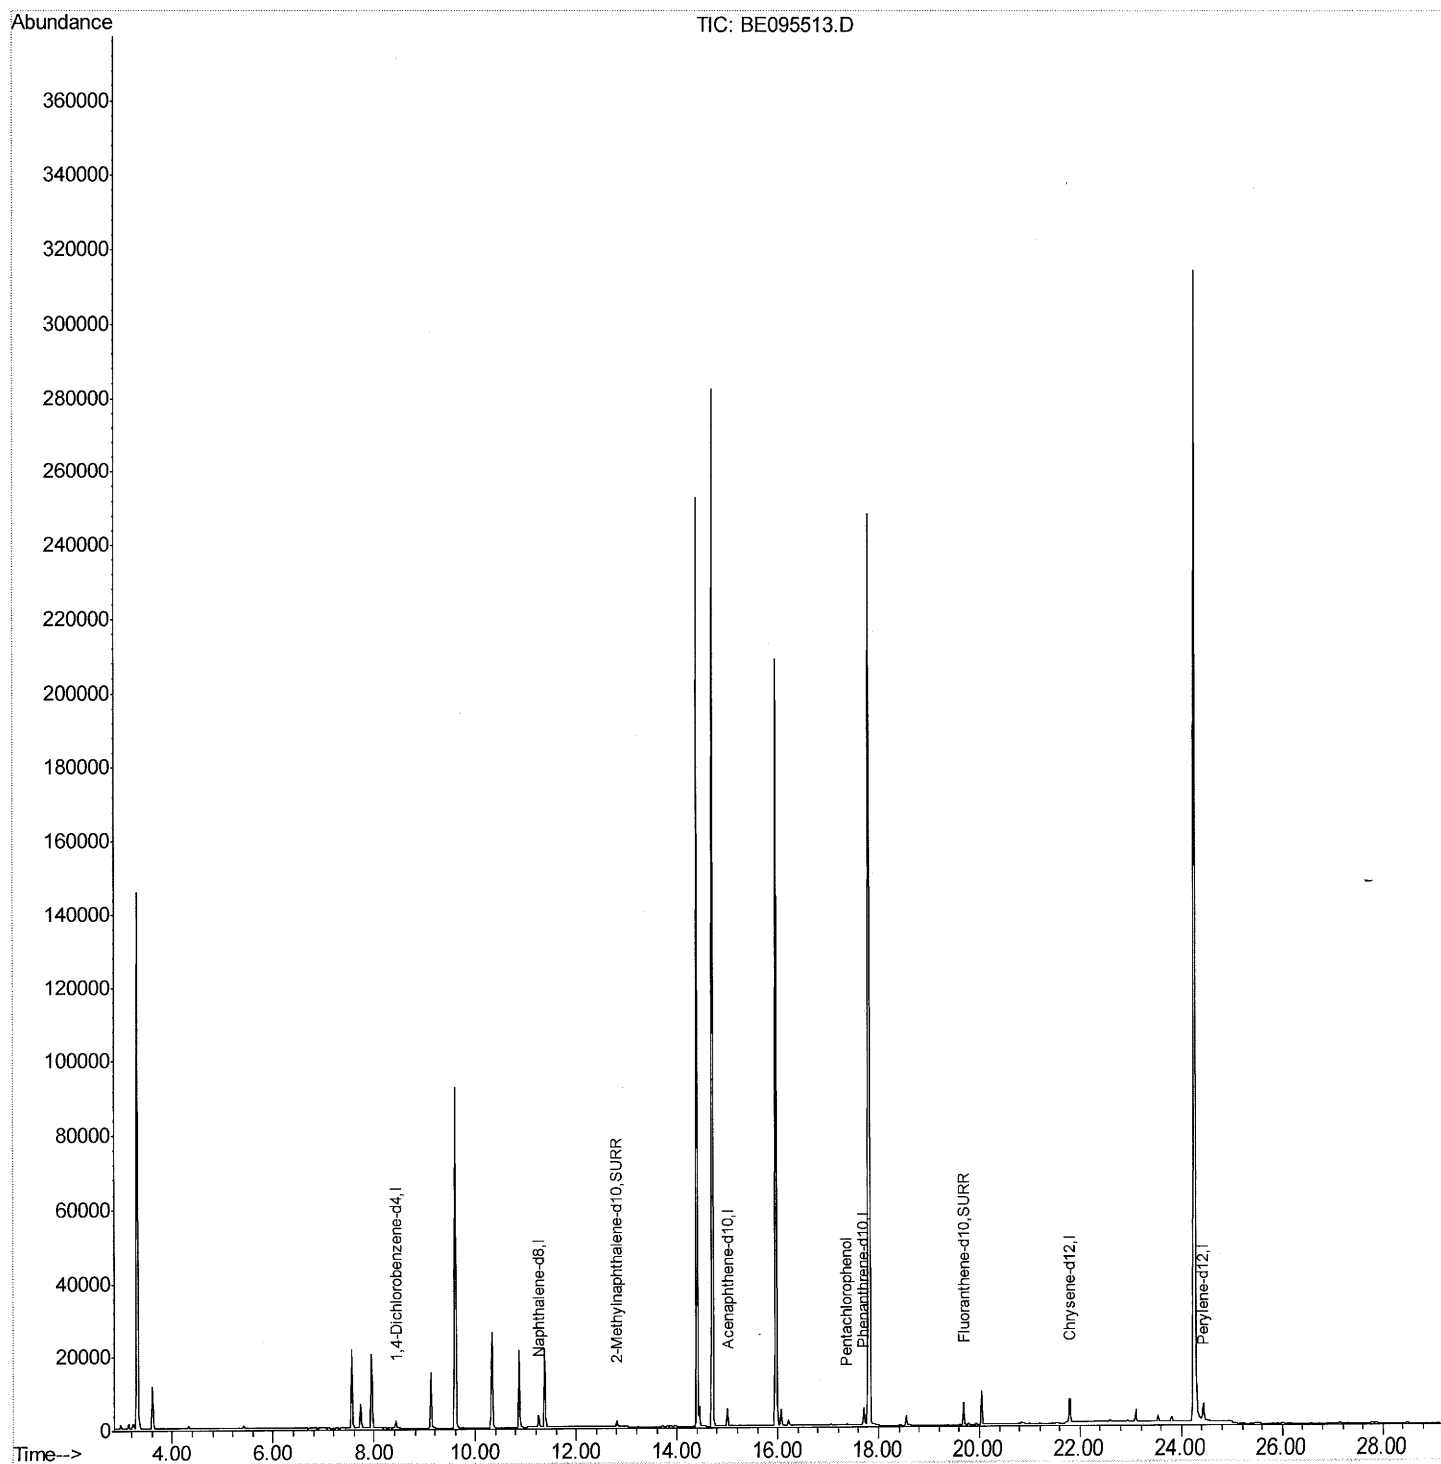

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095513.D
 Acq On : 6 Feb 2018 4:31
 Operator : SJ/JU
 Sample : J1315-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C59

Manual Integrations
 APPROVED

Sohil
 2/6/2018 2:31:42 PM

Quant Time: Feb 06 05:56:28 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 04:22:42 2018
 Response via : Initial Calibration

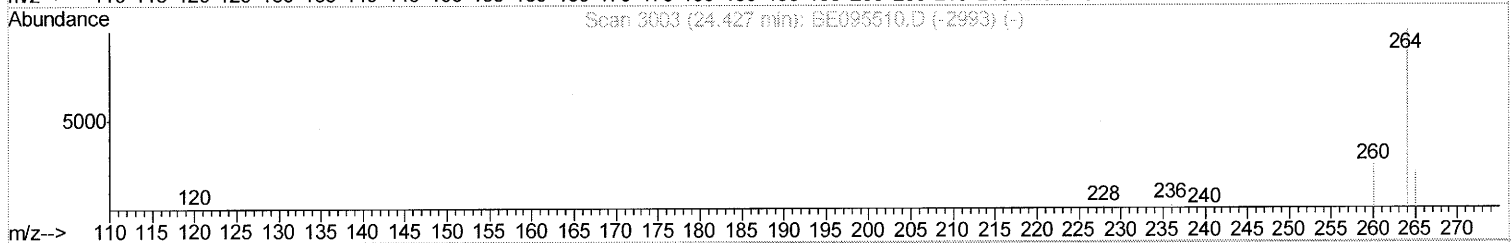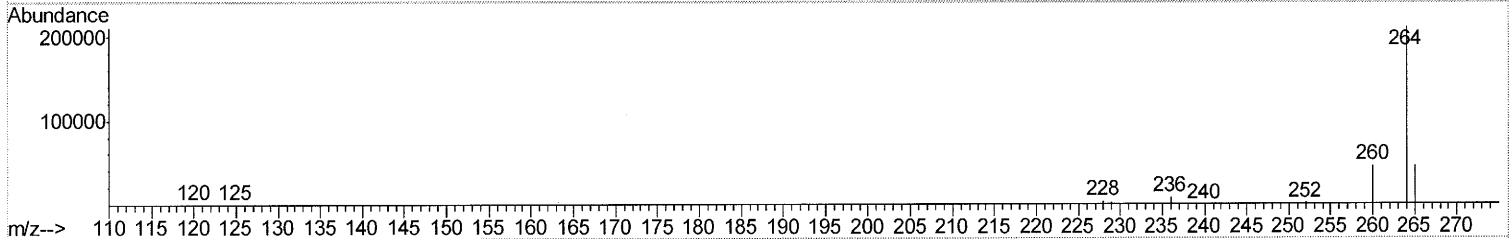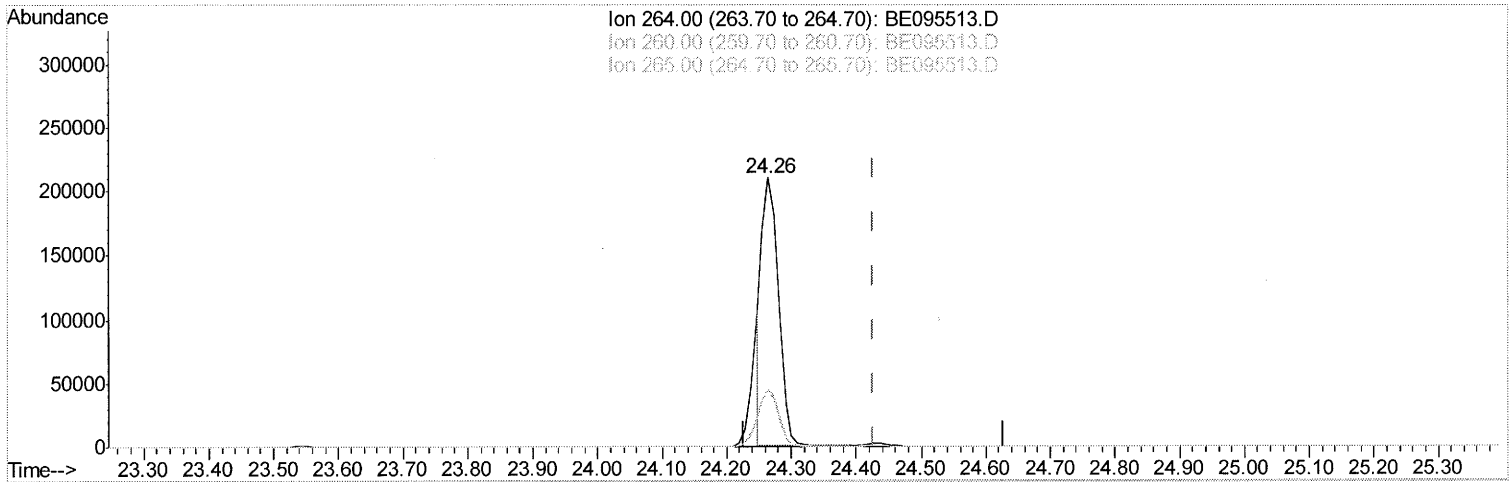

TIC: BE095513.D

(20) Perylene-d12 (I)

24.265min (-0.163) 0.40ng/ul

response 381410

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.33#
265.00	103.50	21.25#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095513.D
Acq On : 6 Feb 2018 4:31
Operator : SJ/JU
Sample : J1315-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6C59

Manual Integrations
APPROVED

Sohil
2/6/2018 2:31:42 PM

Quant Time: Feb 06 05:56:28 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

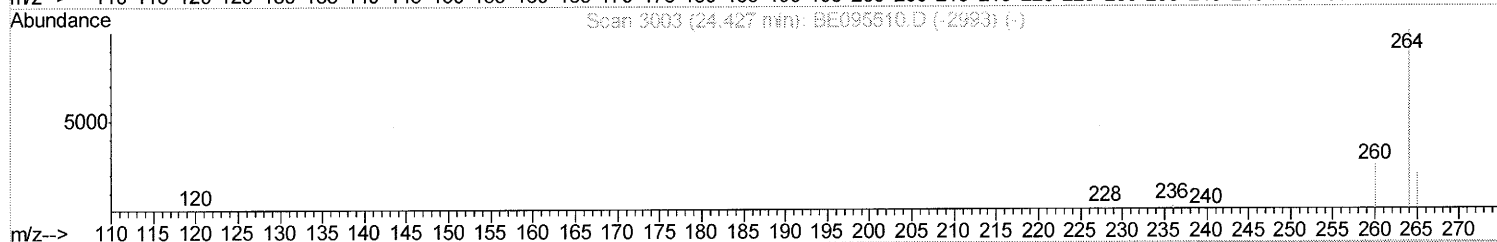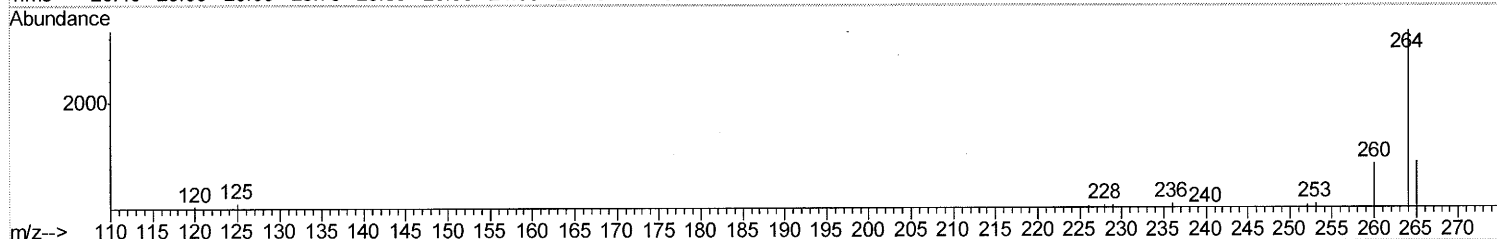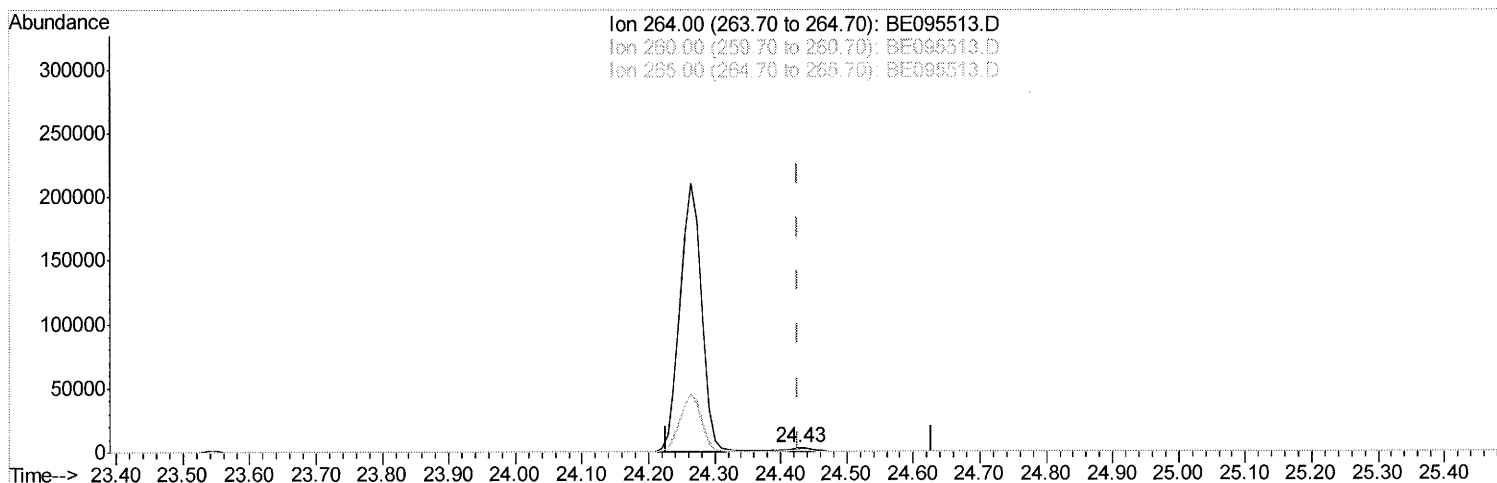

TIC: BE095513.D

(20) Perylene-d12 (I)

24.427min (-0.000) 0.40ng/ul m

response 6639

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.45
265.00	103.50	27.51#
0.00	0.00	0.00

SJ 2/7/18

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095513.D
 Acq On : 6 Feb 2018 4:31
 Operator : SJ/JU
 Sample : J1315-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C59

Manual Integrations
 APPROVED

Sohil
 2/6/2018 2:31:42 PM

Quant Time: Feb 06 06:24:06 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 04:22:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1700	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	4703	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3014	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7022	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6985	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	6639m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2381	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7044	0.26	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	160	0.118	ng/ul	Ovalue 90

SJ 2/7/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed