


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095514.D
Acq On : 6 Feb 2018 5:07
Operator : SJ/JU
Sample : J1315-10
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C67

Manual Integrations
APPROVED

Sohil
2/6/2018 2:31:46 PM

Quant Time: Feb 06 06:26:21 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

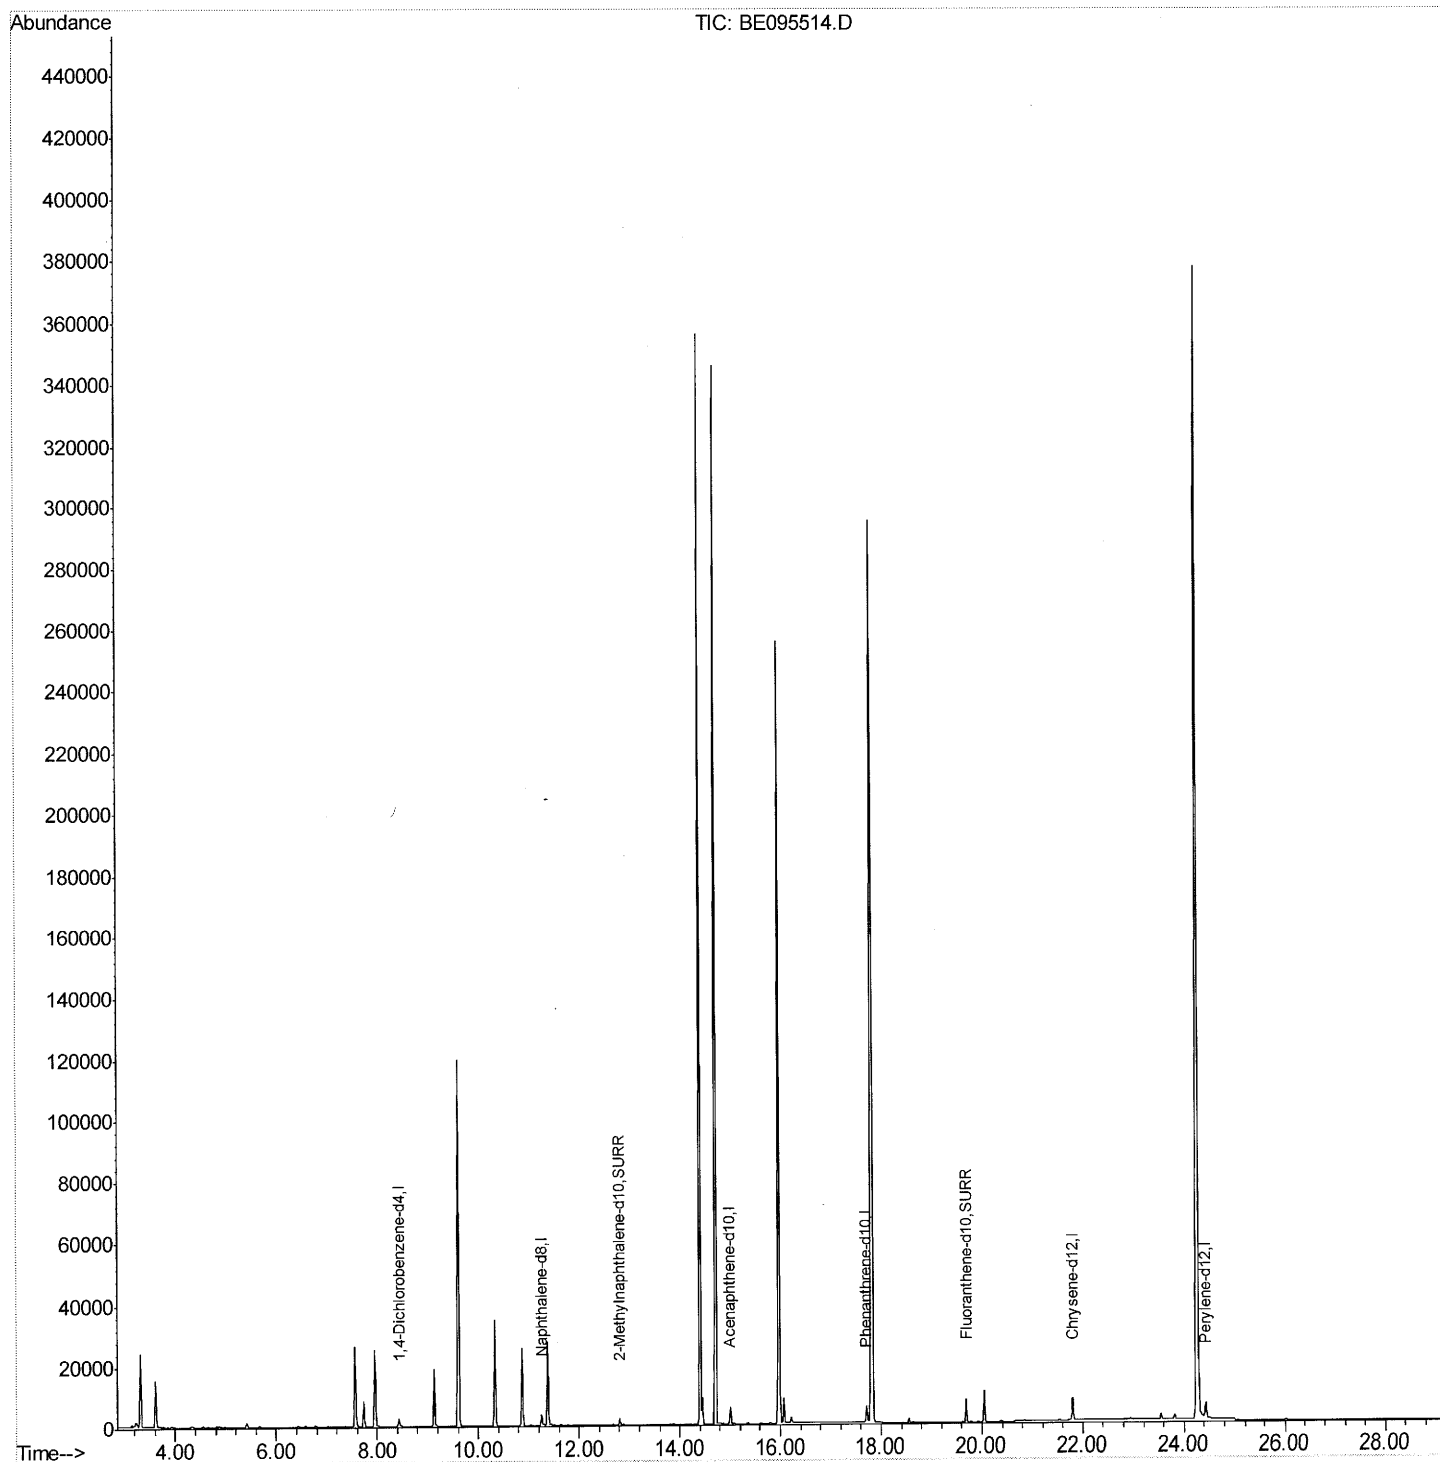

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095514.D
Acq On : 6 Feb 2018 5:07
Operator : SJ/JU
Sample : J1315-10
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6C67

Manual Integrations
APPROVED

Sohil
2/6/2018 2:31:46 PM

Quant Time: Feb 06 05:56:35 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

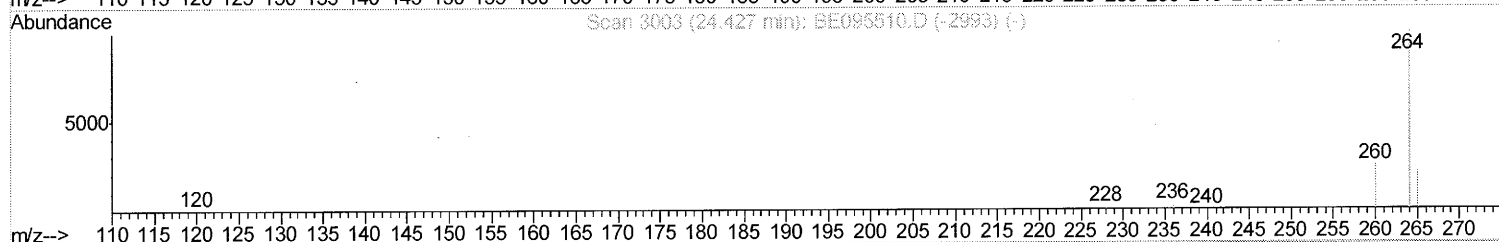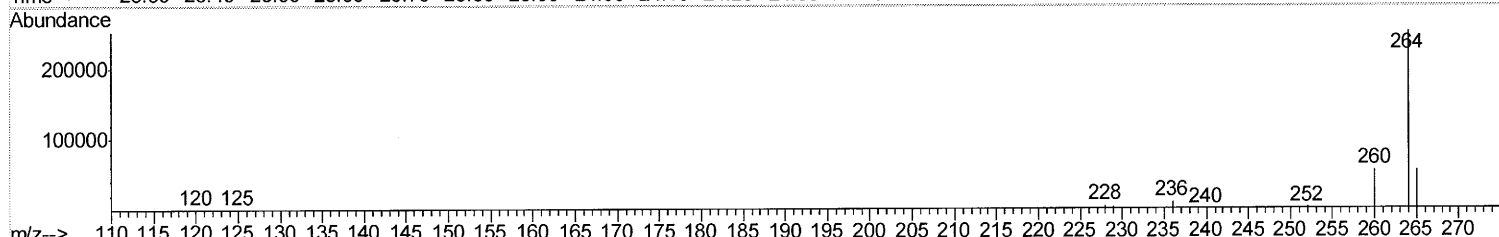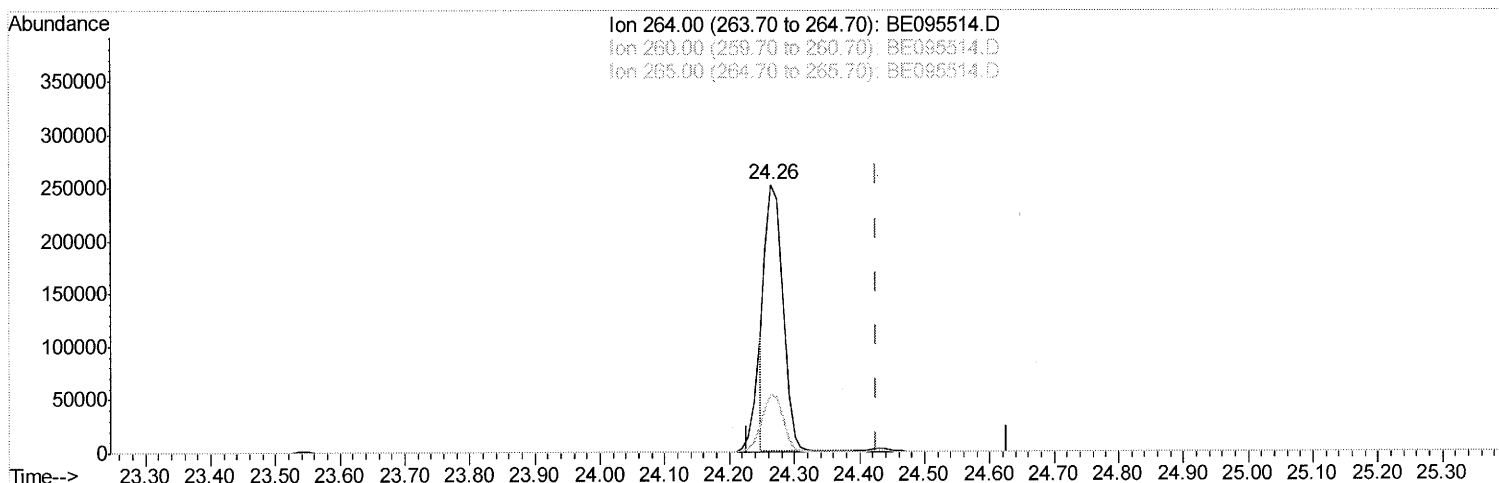

TIC: BE095514.D

(20) Perylene-d12 (I)

24.265min (-0.162) 0.40ng/ul

response 484471

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.42#
265.00	103.50	21.28#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
 Data File : BE095514.D
 Acq On : 6 Feb 2018 5:07
 Operator : SJ/JU
 Sample : J1315-10
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C67

Manual Integrations
 APPROVED

Sohil
 2/6/2018 2:31:46 PM

Quant Time: Feb 06 05:56:35 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 04:22:42 2018
 Response via : Initial Calibration

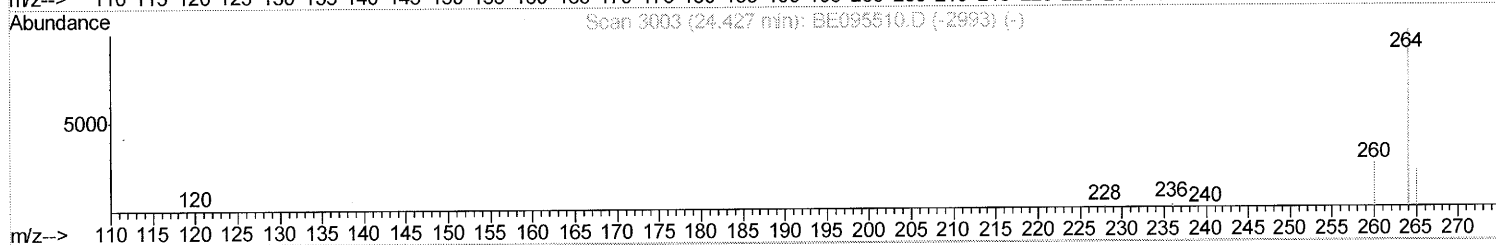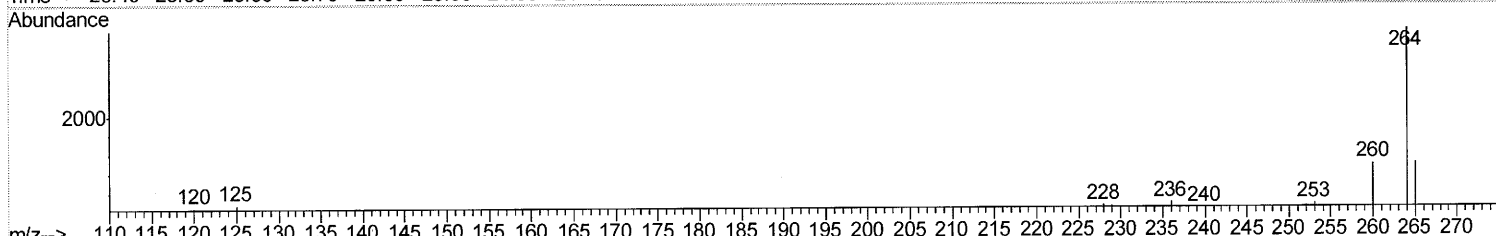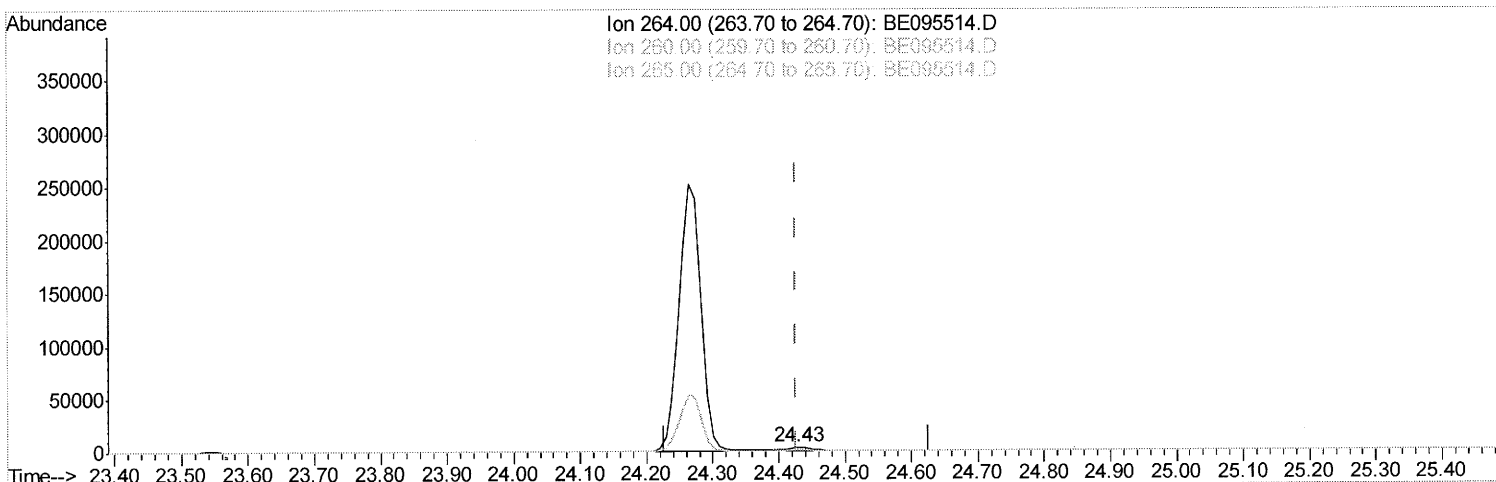

TIC: BE095514.D

(20) Perylene-d12 (I)

24.427min (-0.000) 0.40ng/ul m

response 7310

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.48
265.00	103.50	26.18#
0.00	0.00	0.00

SJ 2/7/18

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095514.D
Acq On : 6 Feb 2018 5:07
Operator : SJ/JU
Sample : J1315-10
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C67

Manual Integrations
APPROVED

Sohil
2/6/2018 2:31:46 PM

Quant Time: Feb 06 06:26:21 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1896	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5401	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3431	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7900	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7893	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7310m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	3004	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8633	0.29	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ 2/7/18