


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095519.D
Acq On : 6 Feb 2018 8:03
Operator : SJ/JU
Sample : PB106182BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
SBLK82

Manual Integrations
APPROVED

Sohil
2/6/2018 2:32:44 PM

Quant Time: Feb 06 08:43:23 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

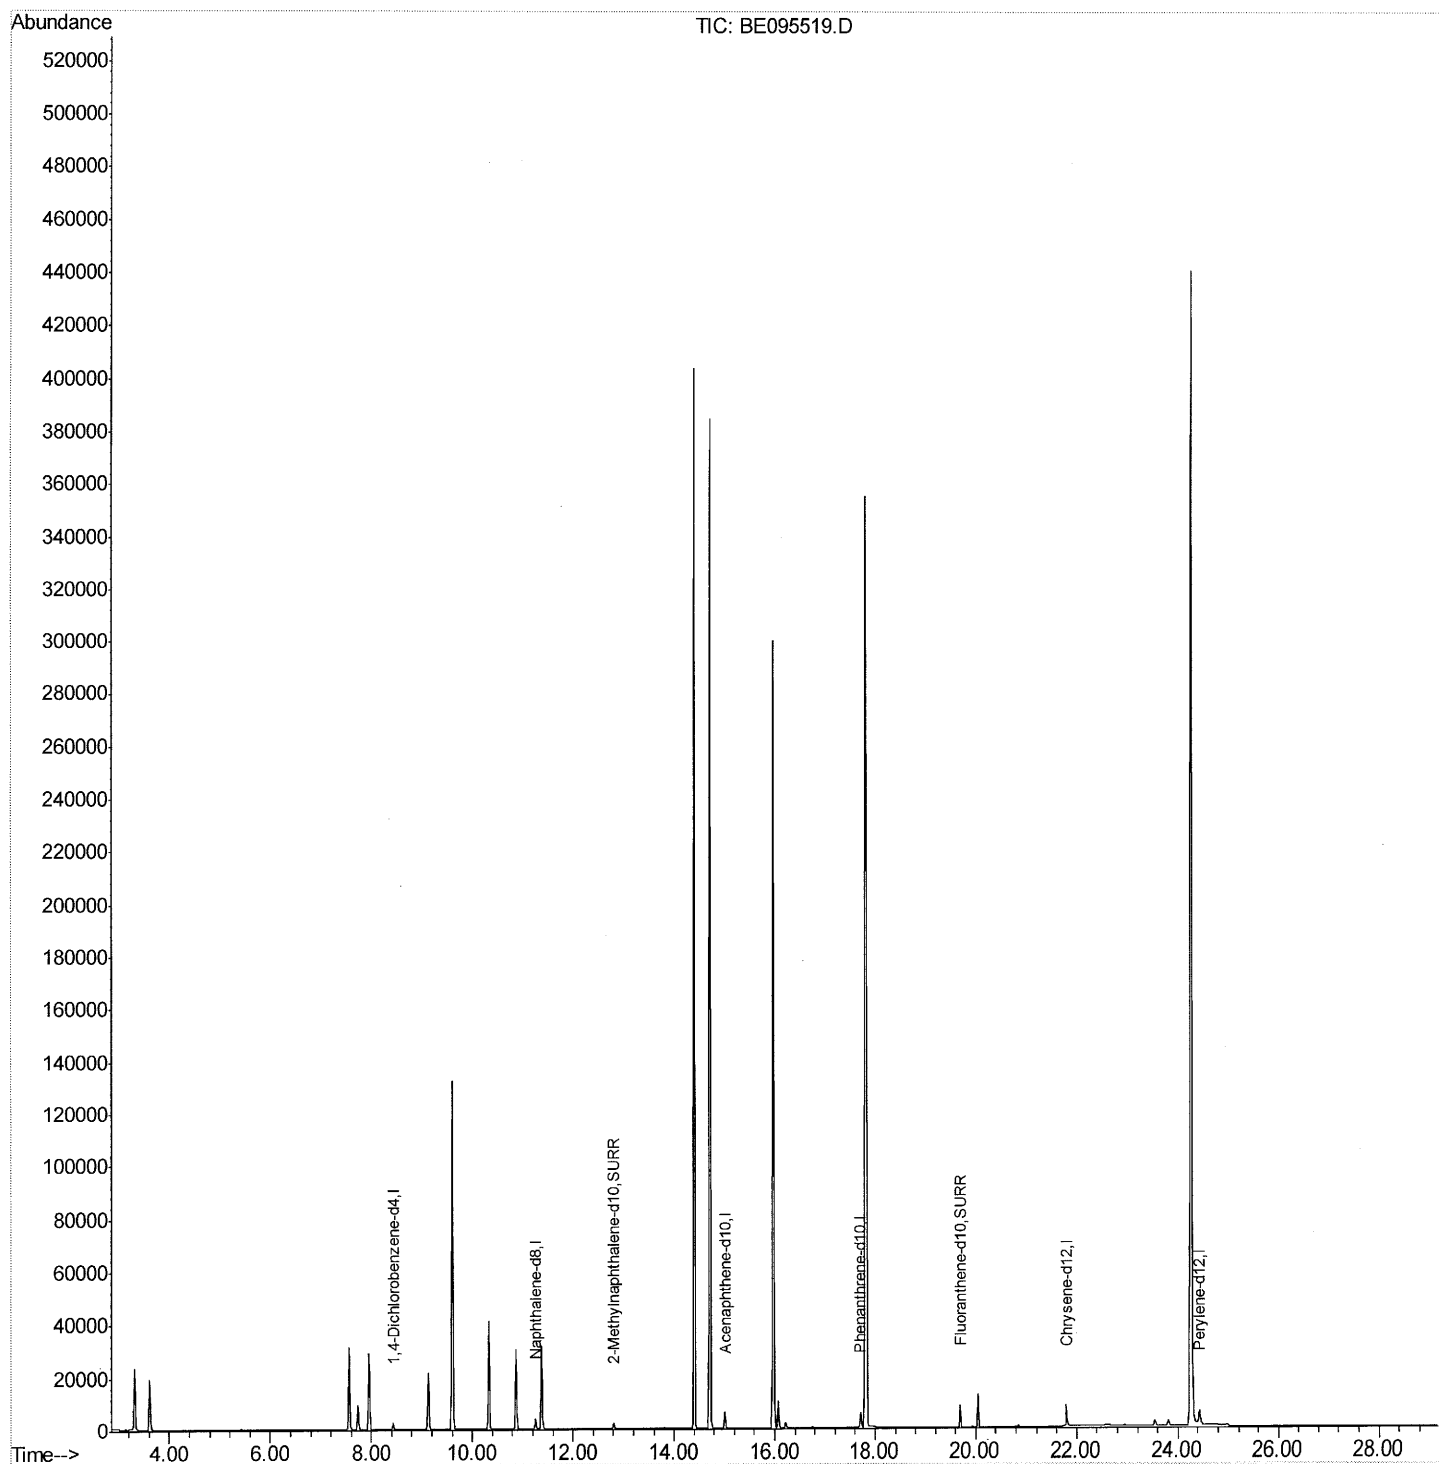

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095519.D
Acq On : 6 Feb 2018 8:03
Operator : SJ/JU
Sample : PB106182BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
SBLK82

Manual Integrations
APPROVED

Sohil
2/6/2018 2:32:44 PM

Quant Time: Feb 06 08:41:55 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

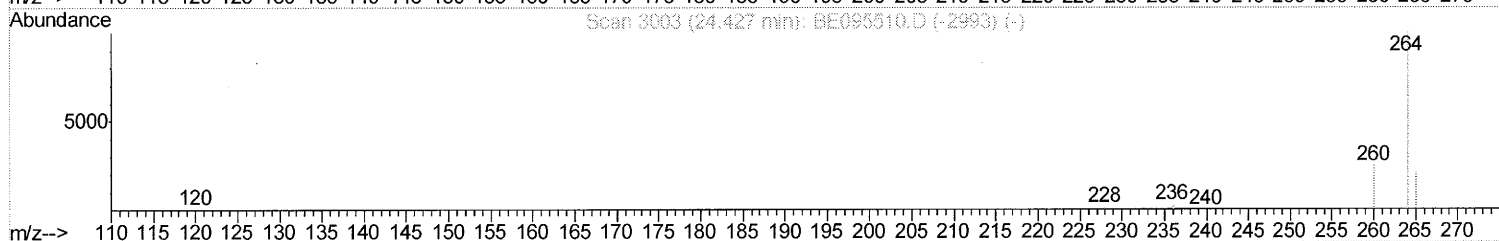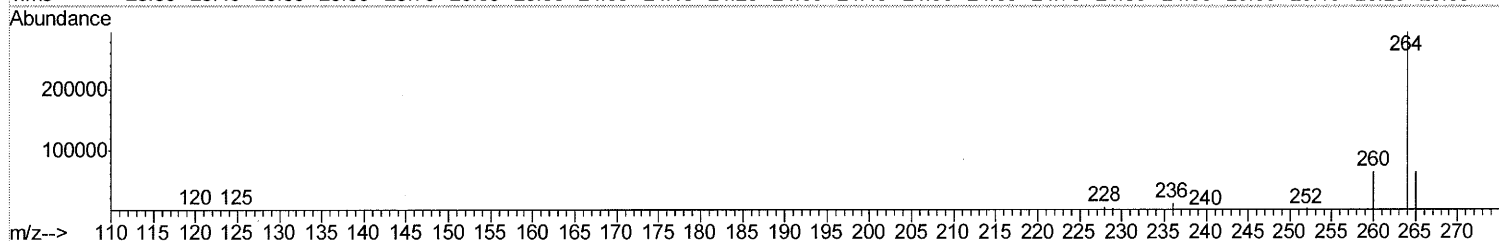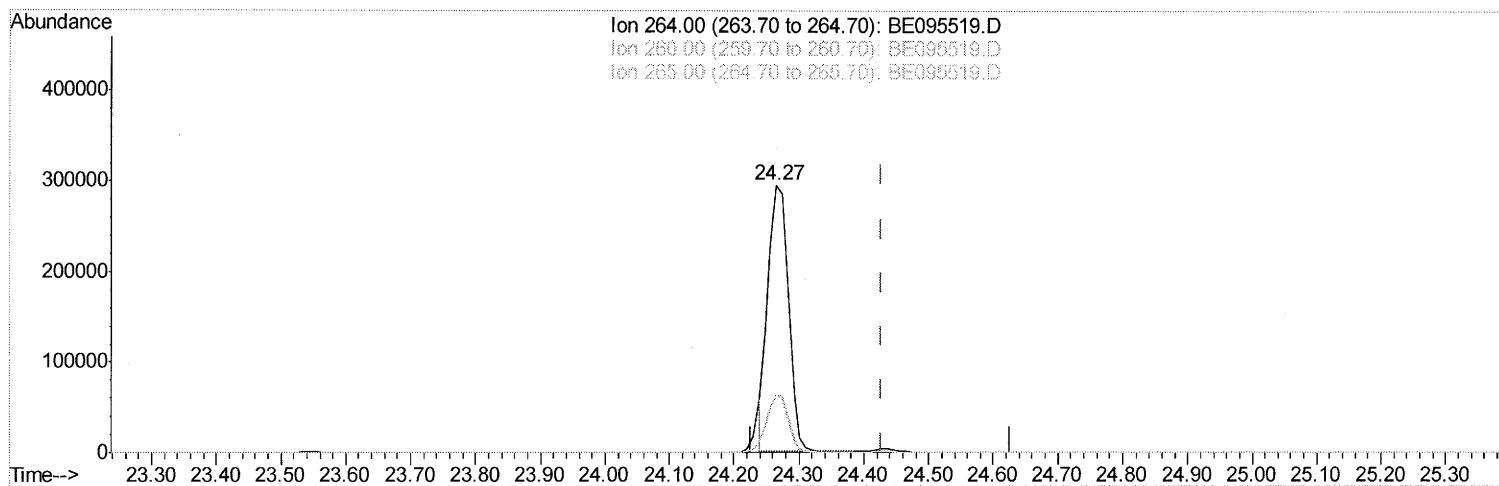

TIC: BE095519.D

(20) Perylene-d12 (I)

24.265min (-0.162) 0.40ng/ul

response 650385

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.40#
265.00	103.50	21.23#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095519.D
Acq On : 6 Feb 2018 8:03
Operator : SJ/JU
Sample : PB106182BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_E
Client Sampled :
SBLK82

Manual Integrations
APPROVED

Sohil
2/6/2018 2:32:44 PM

Quant Time: Feb 06 08:41:55 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

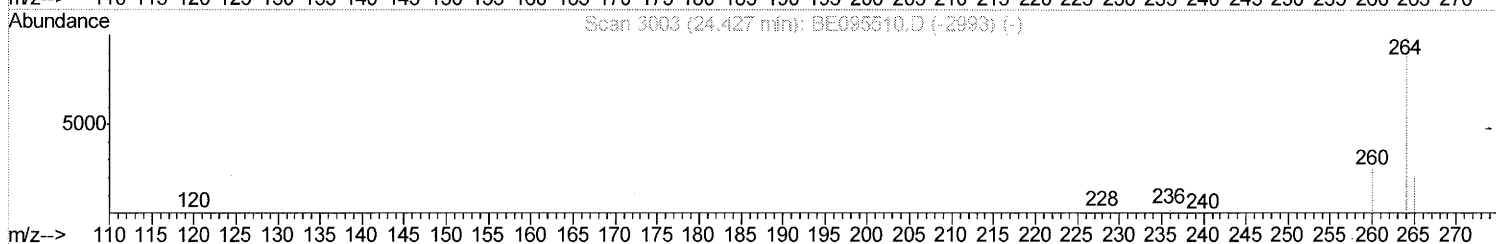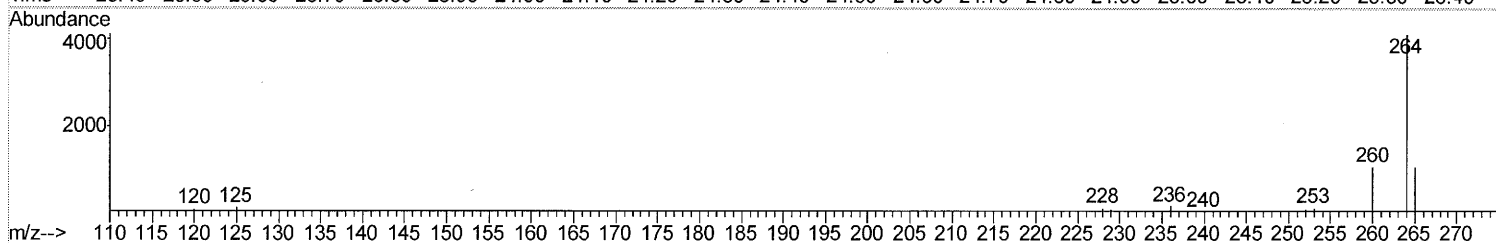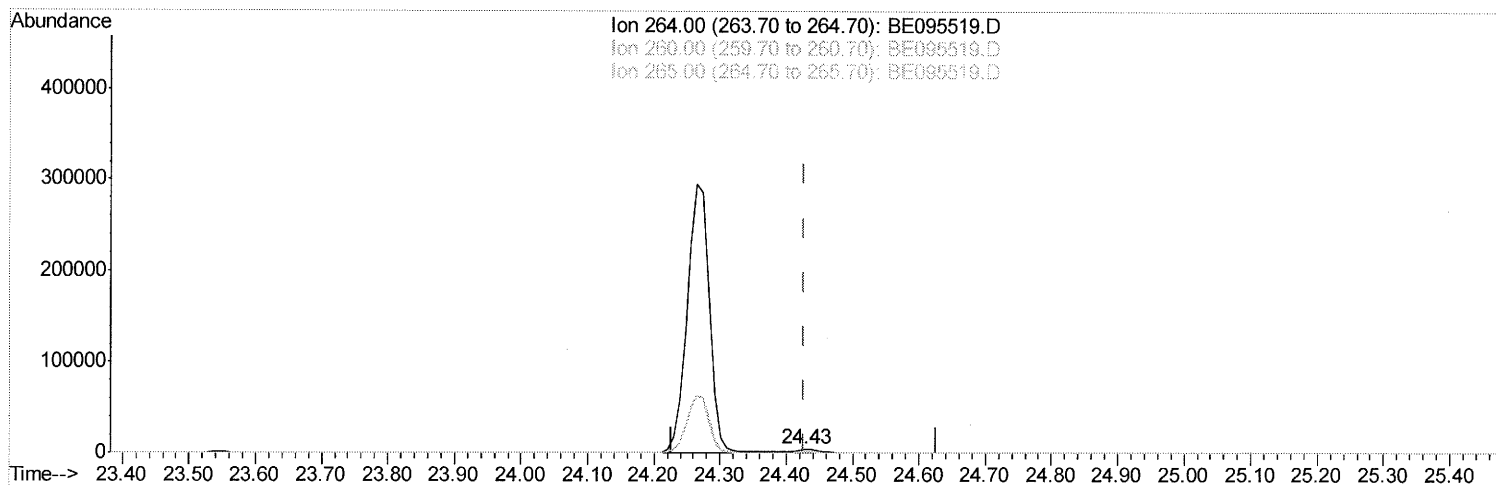

TIC: BE095519.D

(20) Perylene-d12 (I)

24.428min (+0.001) 0.40ng/ul m

response 8221

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.83
265.00	103.50	25.93#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020518\
Data File : BE095519.D
Acq On : 6 Feb 2018 8:03
Operator : SJ/JU
Sample : PB106182BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
SBLK82

Manual Integrations
APPROVED

Sohil
2/6/2018 2:32:44 PM

Quant Time: Feb 06 08:43:23 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	2003	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5822	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3729	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8532	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8596	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	8221m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.81	152	3370	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9934	0.30	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ 2/7/18