


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095520.D
Acq On : 6 Feb 2018 8:39
Operator : SJ/JU
Sample : PB106191BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
SBLK91

Manual Integrations
APPROVED

Sohil
2/6/2018 2:32:48 PM

Quant Time: Feb 06 10:46:47 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

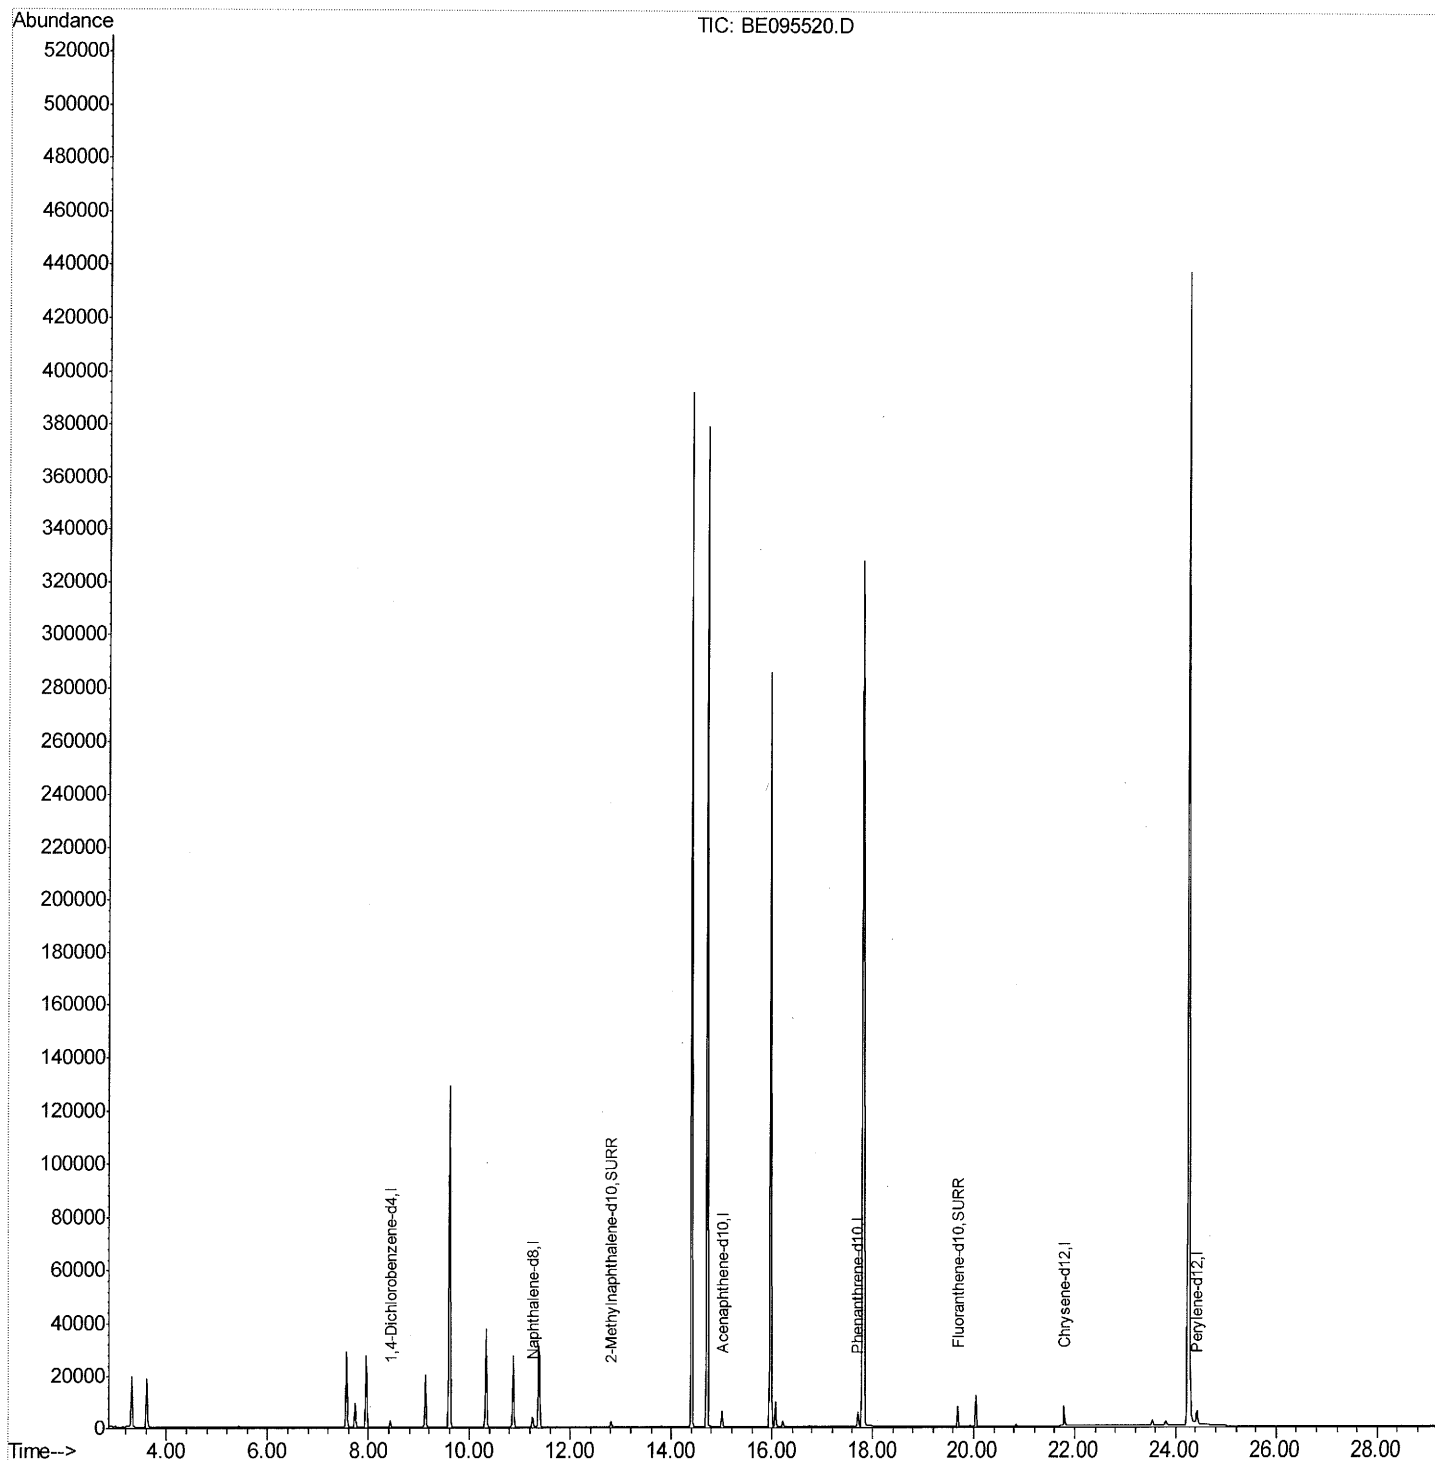

Quantitation Report (Qedit)




Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_E\DATA\BE020518\
 Data File : BE095520.D
 Acq On : 6 Feb 2018 8:39
 Operator : SJ/JU
 Sample : PB106191BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK91

Manual Integrations
 APPROVED

Sohil
 2/6/2018 2:32:48 PM

Quant Time: Feb 06 10:41:02 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 04:22:42 2018
 Response via : Initial Calibration

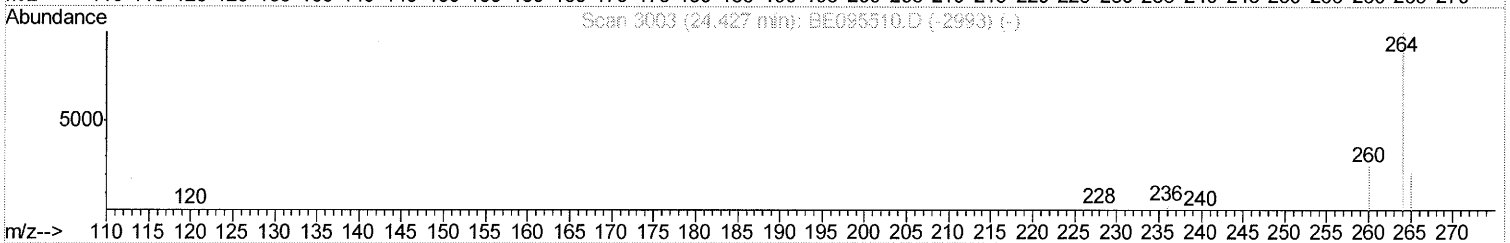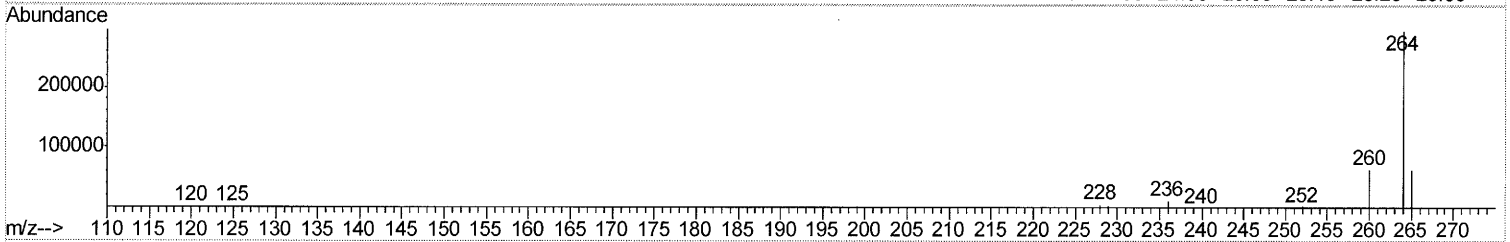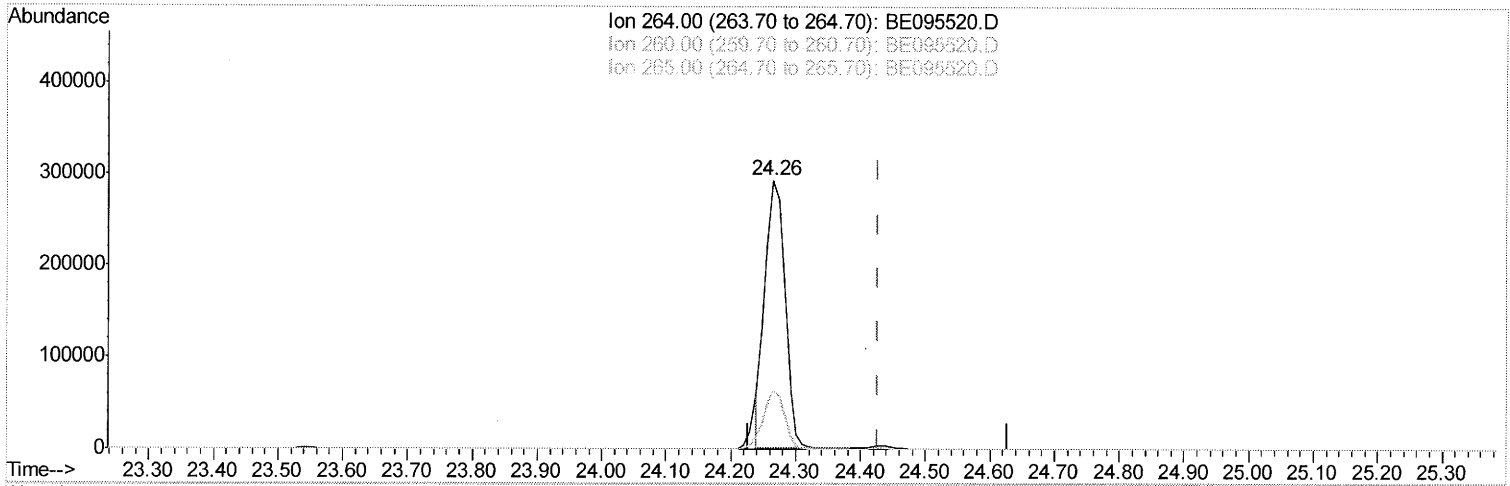

TIC: BE095520.D

(20) Perylene-d12 (I)
 24.265min (-0.162) 0.40ng/ul
 response 628996

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.48#
265.00	103.50	21.28#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_E\DATA\BE020518\
 Data File : BE095520.D
 Acq On : 6 Feb 2018 8:39
 Operator : SJ/JU
 Sample : PB106191BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK91

Manual Integrations
 APPROVED

Sohil
 2/6/2018 2:32:48 PM

Quant Time: Feb 06 10:41:02 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 04:22:42 2018
 Response via : Initial Calibration

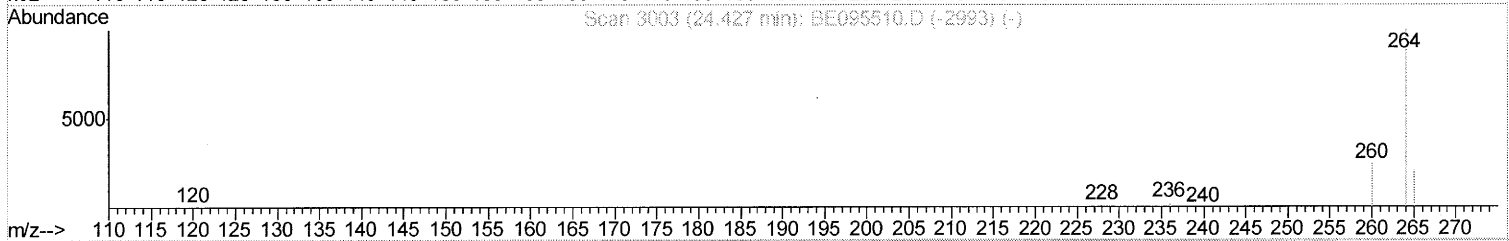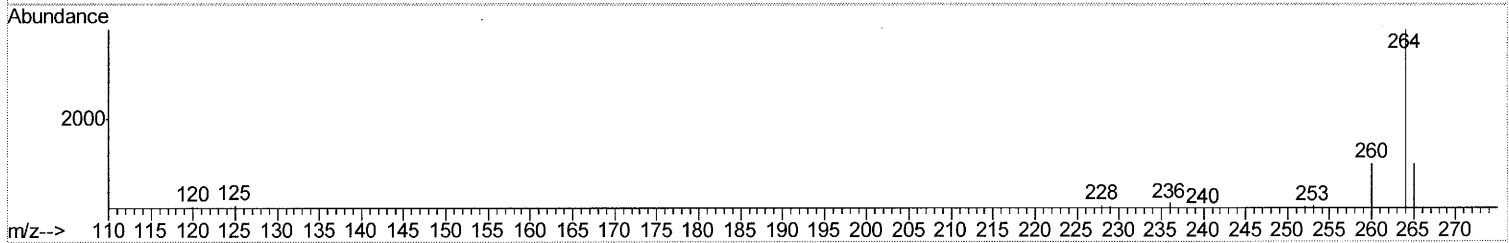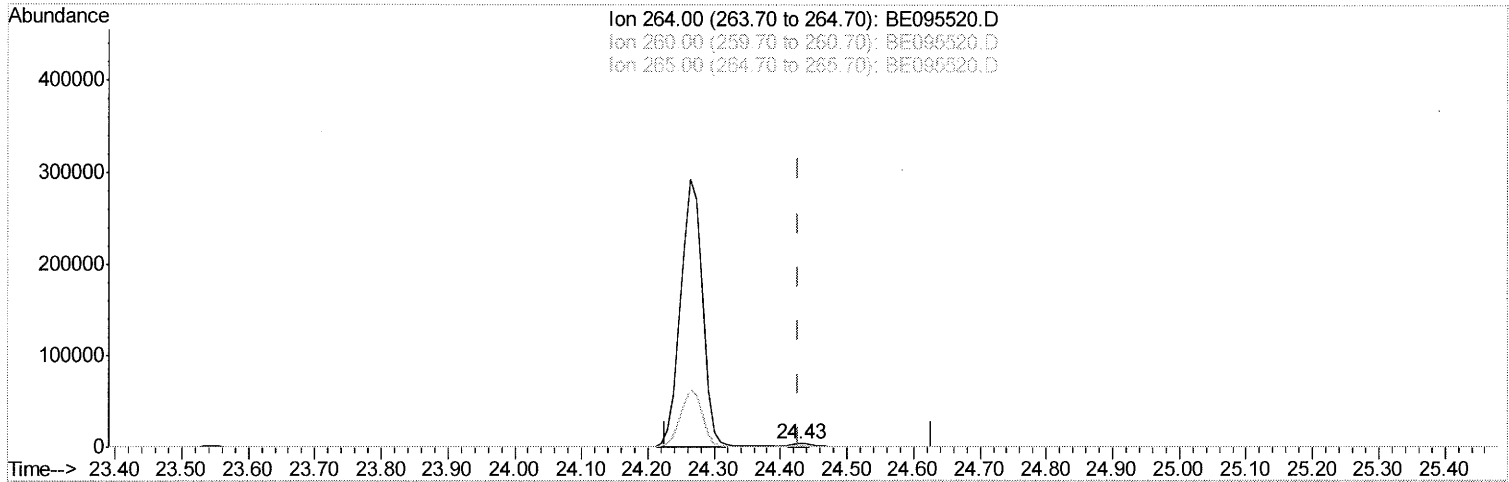

TIC: BE095520.D

(20) Perylene-d12 (I)

24.427min (-0.000) 0.40ng/ul m

SJ 2/7/18

response 7076

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.02
265.00	103.50	25.80#
0.00	0.00	0.00

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095520.D
Acq On : 6 Feb 2018 8:39
Operator : SJ/JU
Sample : PB106191BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
SBLK91

Manual Integrations
APPROVED

Sohil
2/6/2018 2:32:48 PM

Quant Time: Feb 06 10:46:47 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1936	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5526	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3537	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8340	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8212	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7076m	0.40	ng/ul	0.00

SJ 2/7/18

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	3143	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9616	0.30	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed