

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095521.D
Acq On : 6 Feb 2018 9:15
Operator : SJ/JU
Sample : J1316-16
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Feb 06 10:41:07 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

Instrument :

BNA_E




ClientSampleId :

F6C96

Manual Integrations
APPROVED

Sohil

2/6/2018 2:32:50 PM

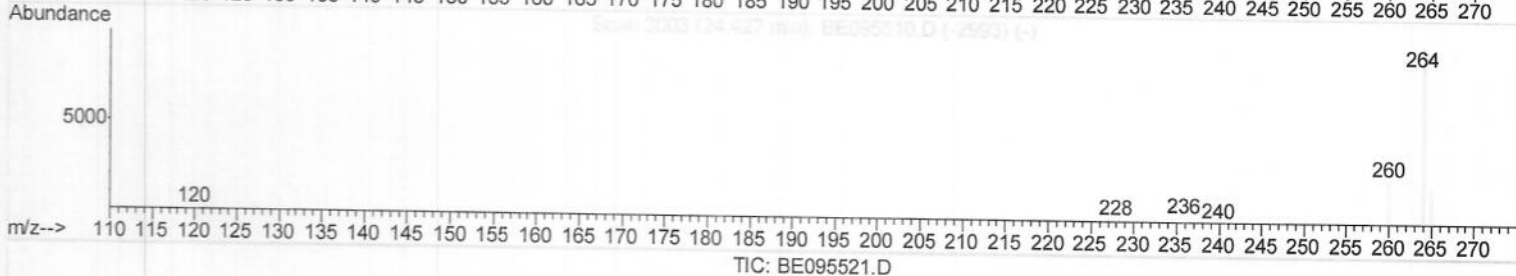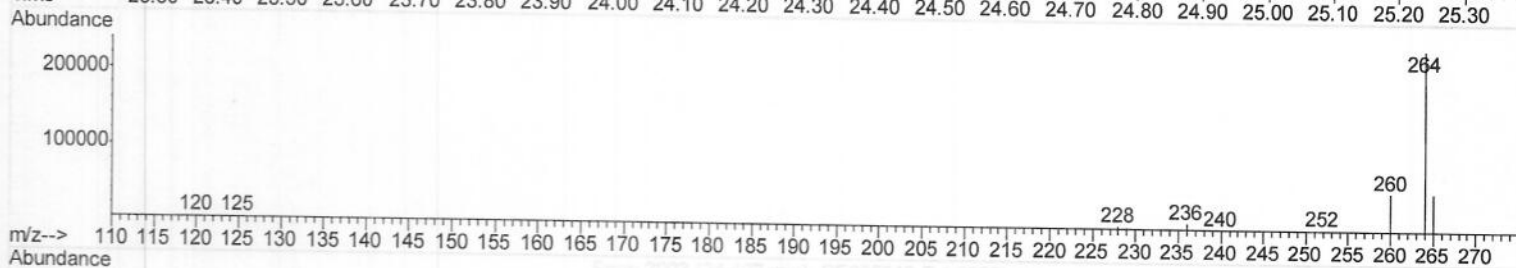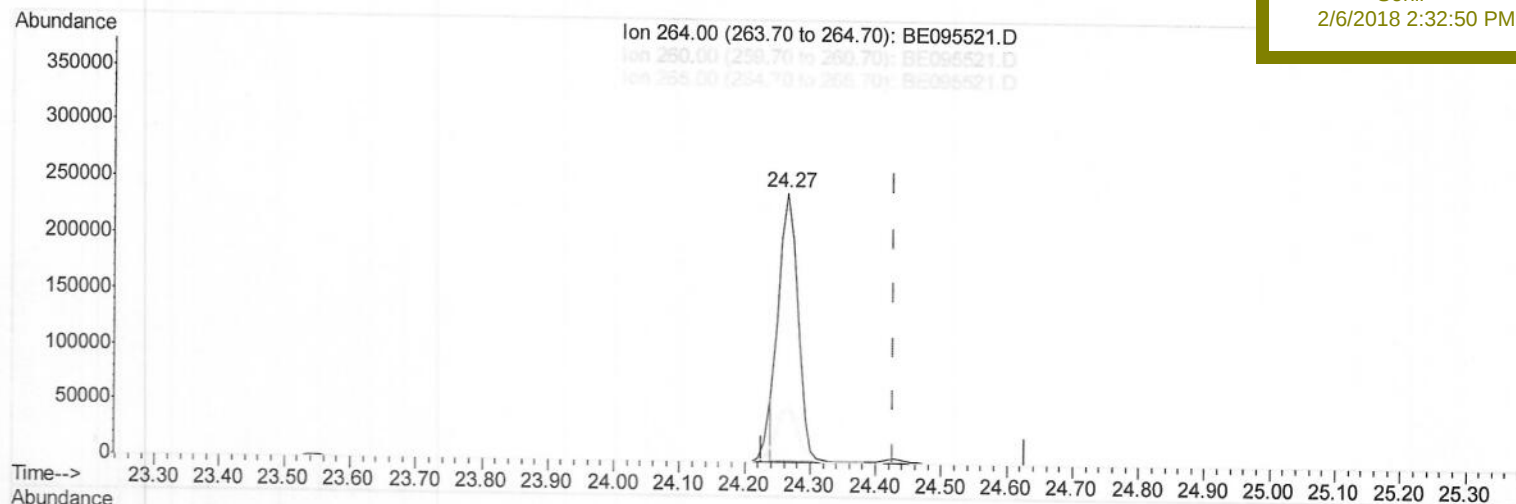

(20) Perylene-d12 (I)

24.265min (-0.162) 0.40ng/ul

response 496003

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.20#
265.00	103.50	21.35#
0.00	0.00	0.00




Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095521.D
Acq On : 6 Feb 2018 9:15
Operator : SJ/JU
Sample : J1316-16
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Feb 06 10:41:07 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
F6C96

Manual Integrations
APPROVED

Sohil
2/6/2018 2:32:50 PM

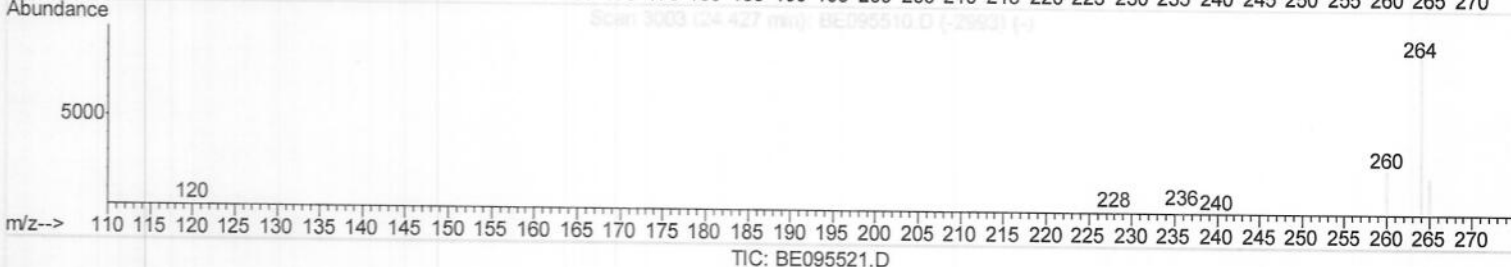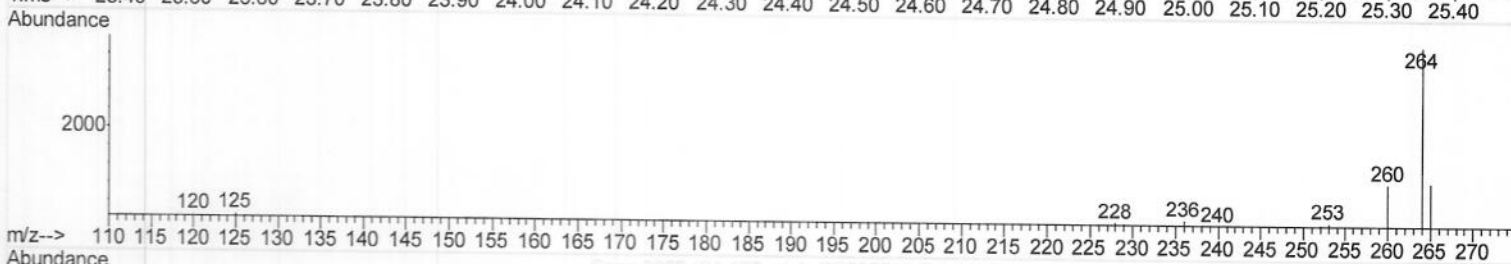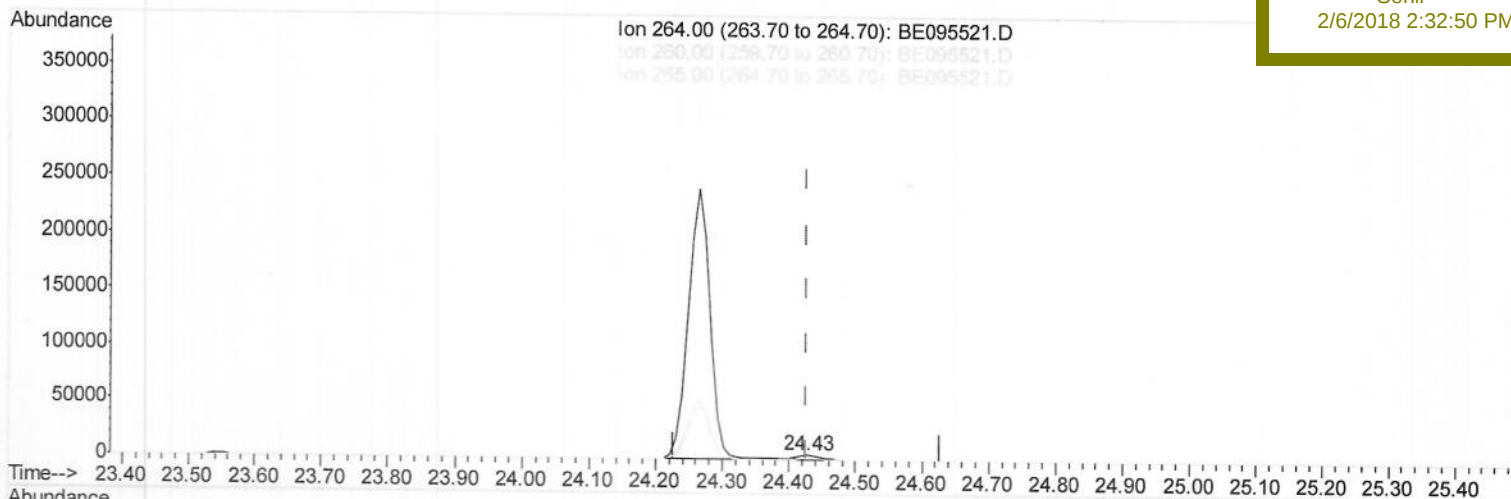

(20) Perylene-d12 (I)

24.427min (+0.000) 0.40ng/ul m) JY 02/14/18

response 7500

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.75
265.00	103.50	25.48#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE020518\

Data File : BE095521.D

Acq On : 6 Feb 2018 9:15

Operator : SJ/JU

Sample : J1316-16

Misc :

ALS Vial : 37 Sample Multiplier: 1

Quant Time: Feb 14 01:27:14 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 06 04:22:42 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6C96

Manual Integrations

APPROVED

Sohil

2/6/2018 2:32:50 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1935	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5705	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3630	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8163	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8302	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7500m)	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2717	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7988	0.26	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\Data\BE020518\
Data File : BE095521.D
Acq On : 6 Feb 2018 9:15
Operator : SJ/JU
Sample : J1316-16
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Feb 14 01:27:14 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
F6C96

Manual Integrations
APPROVED

Sohil
2/6/2018 2:32:50 PM

