


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095522.D
Acq On : 6 Feb 2018 9:51
Operator : SJ/JU
Sample : J1317-13
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6D06

Manual Integrations
APPROVED

Sohil
2/6/2018 2:32:52 PM

Quant Time: Feb 06 10:56:59 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

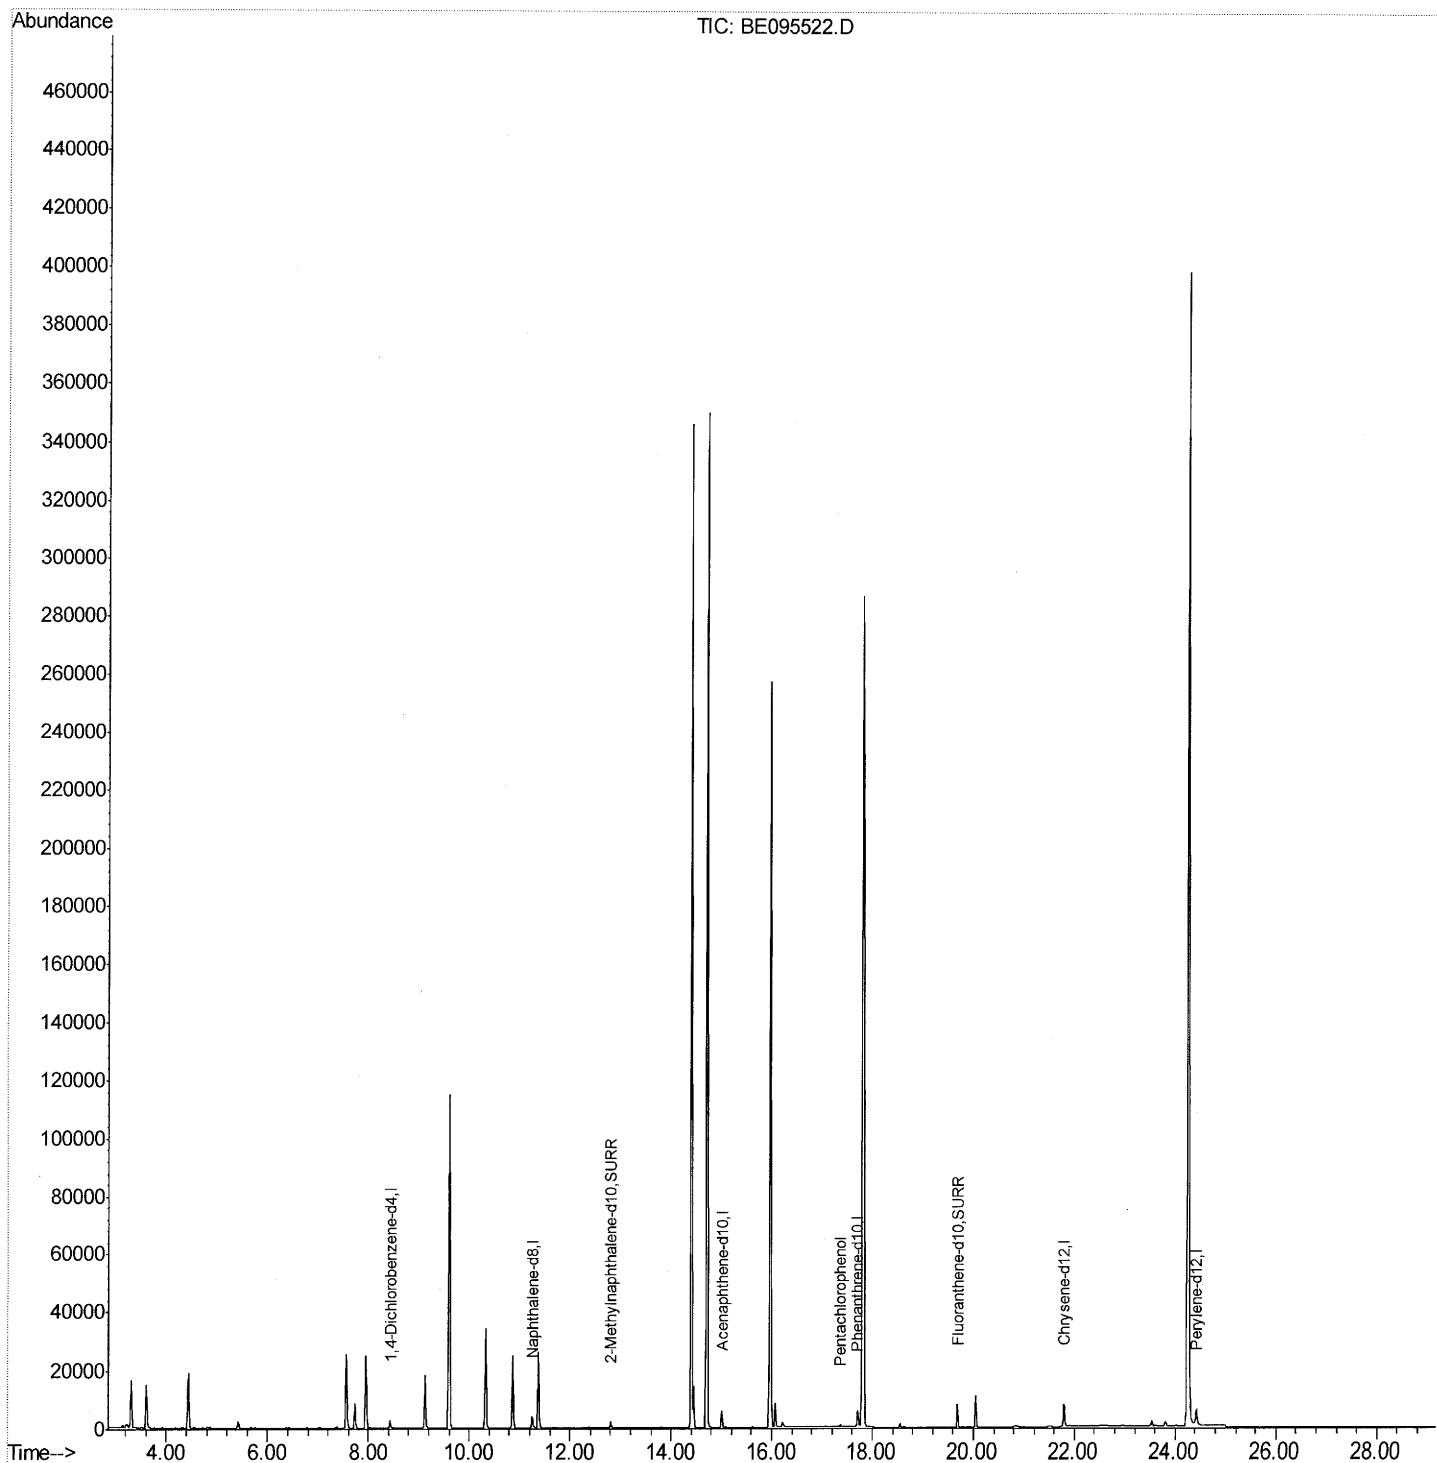

Quantitation Report (Qedit)




Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_E\DATA\BE020518\
 Data File : BE095522.D
 Acq On : 6 Feb 2018 9:51
 Operator : SJ/JU
 Sample : J1317-13
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6D06

Manual Integrations
 APPROVED

Sohil
 2/6/2018 2:32:52 PM

Quant Time: Feb 06 10:41:13 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 04:22:42 2018
 Response via : Initial Calibration

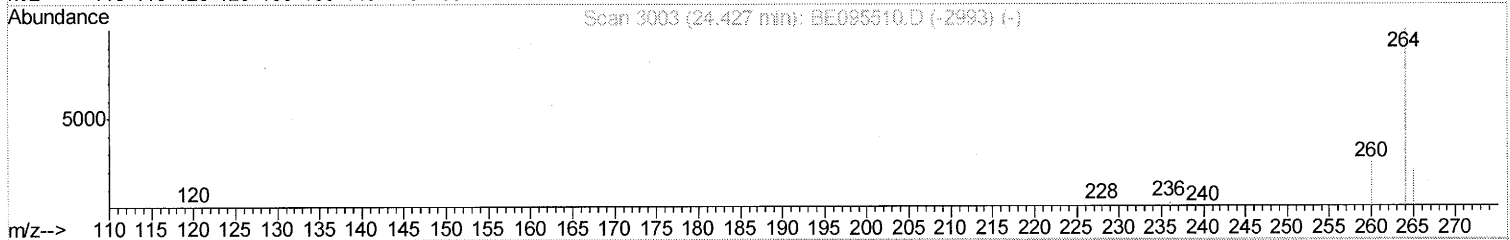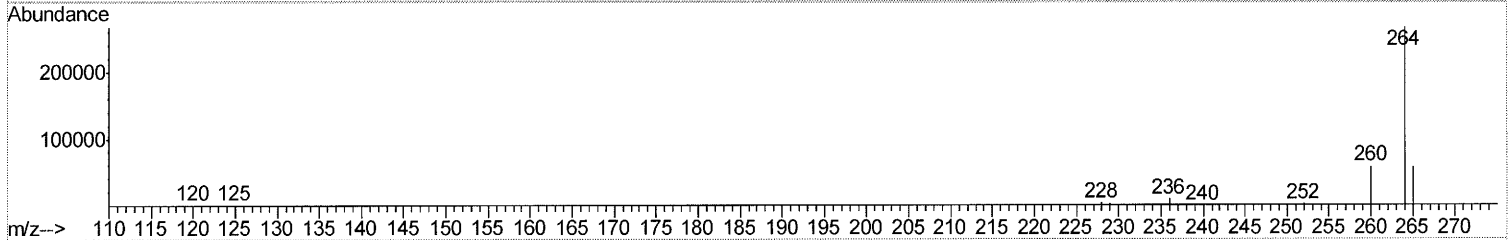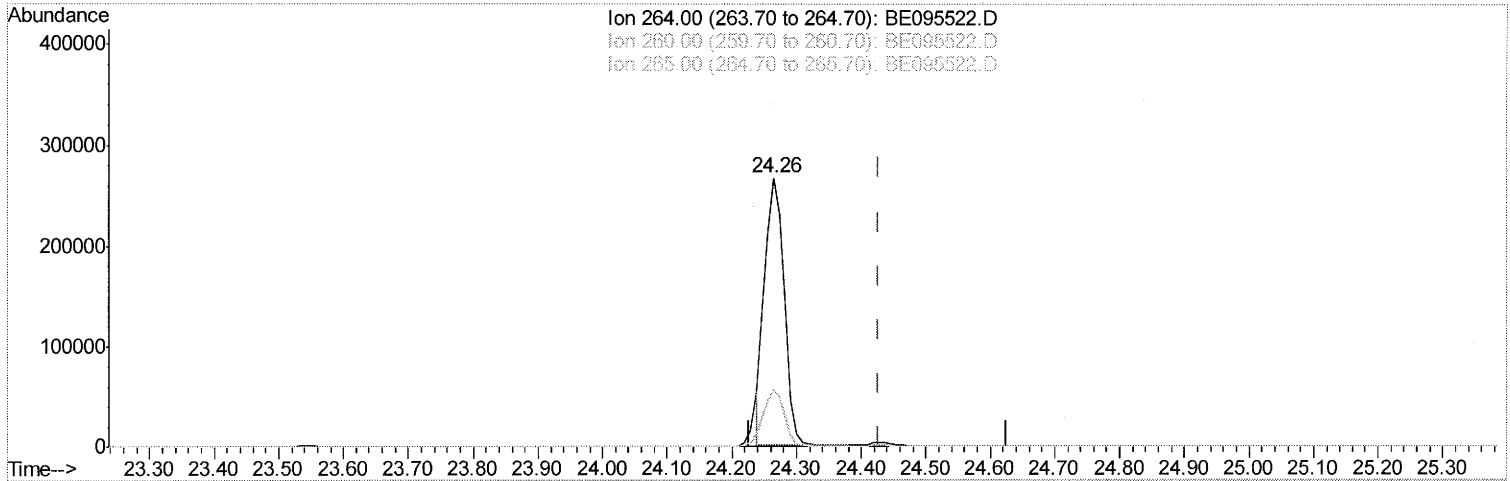

TIC: BE095522.D

(20) Perylene-d12 (I)

24.265min (-0.162) 0.40ng/ul

response 557929

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.35#
265.00	103.50	21.27#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_E\DATA\BE020518\
 Data File : BE095522.D
 Acq On : 6 Feb 2018 9:51
 Operator : SJ/JU
 Sample : J1317-13
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6D06

Manual Integrations
 APPROVED

Sohil
 2/6/2018 2:32:52 PM

Quant Time: Feb 06 10:41:13 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 04:22:42 2018
 Response via : Initial Calibration

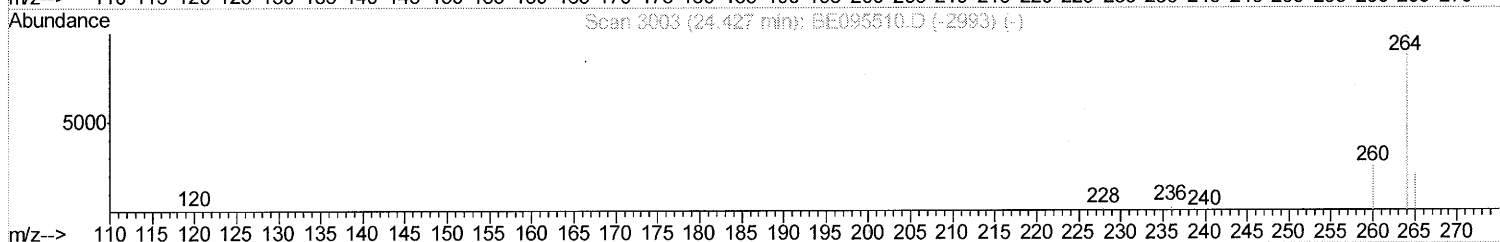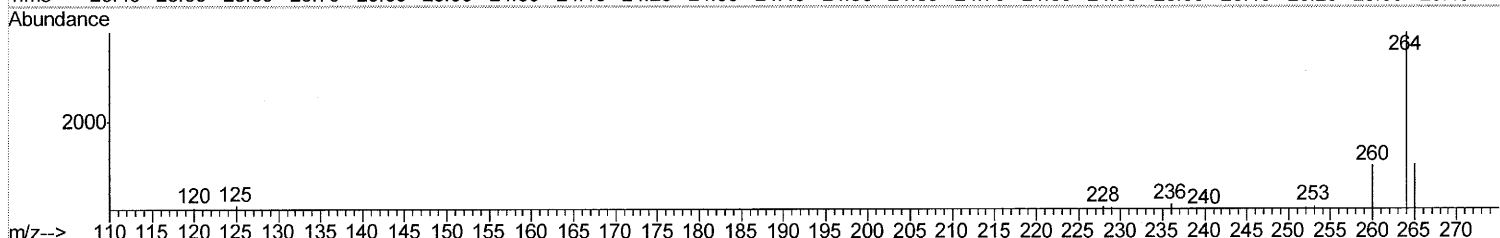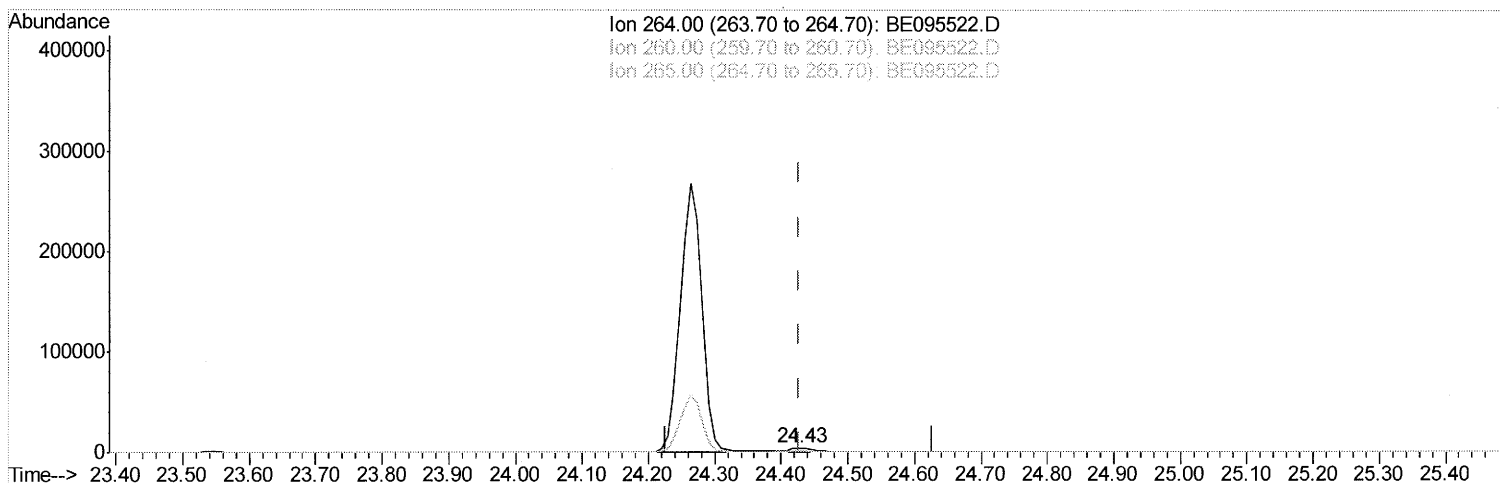

TIC: BE095522.D

(20) Perylene-d12 (I)

24.427min (-0.000) 0.40ng/ul m

SJ 2/7/18

response 7319

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.47
265.00	103.50	26.07#
0.00	0.00	0.00

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095522.D
Acq On : 6 Feb 2018 9:51
Operator : SJ/JU
Sample : J1317-13
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6D06

Manual Integrations
APPROVED

Sohil
2/6/2018 2:32:52 PM

Quant Time: Feb 06 10:56:59 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 04:22:42 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1969	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5650	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3631	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8229	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8190	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7319m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	2873	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8863	0.28	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Pentachlorophenol	17.36	266	531	0.333	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ 2/7/18