

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
 Data File : BE095498.D
 Acq On : 5 Feb 2018 19:37
 Operator : SJ/JU
 Sample : J1296-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C26

Quant Time: Feb 06 02:56:59 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 02:09:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1831	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5163	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3170	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7253	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7623	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	8727	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2487	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7340	0.26	ng/ul	0.00
Target Compounds						
18) Benzo(a)anthracene	21.78	228	548	0.023	ng/ul#	Qvalue 71




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095498.D
Acq On : 5 Feb 2018 19:37
Operator : SJ/JU
Sample : J1296-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C26

Quant Time: Feb 06 02:56:59 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration

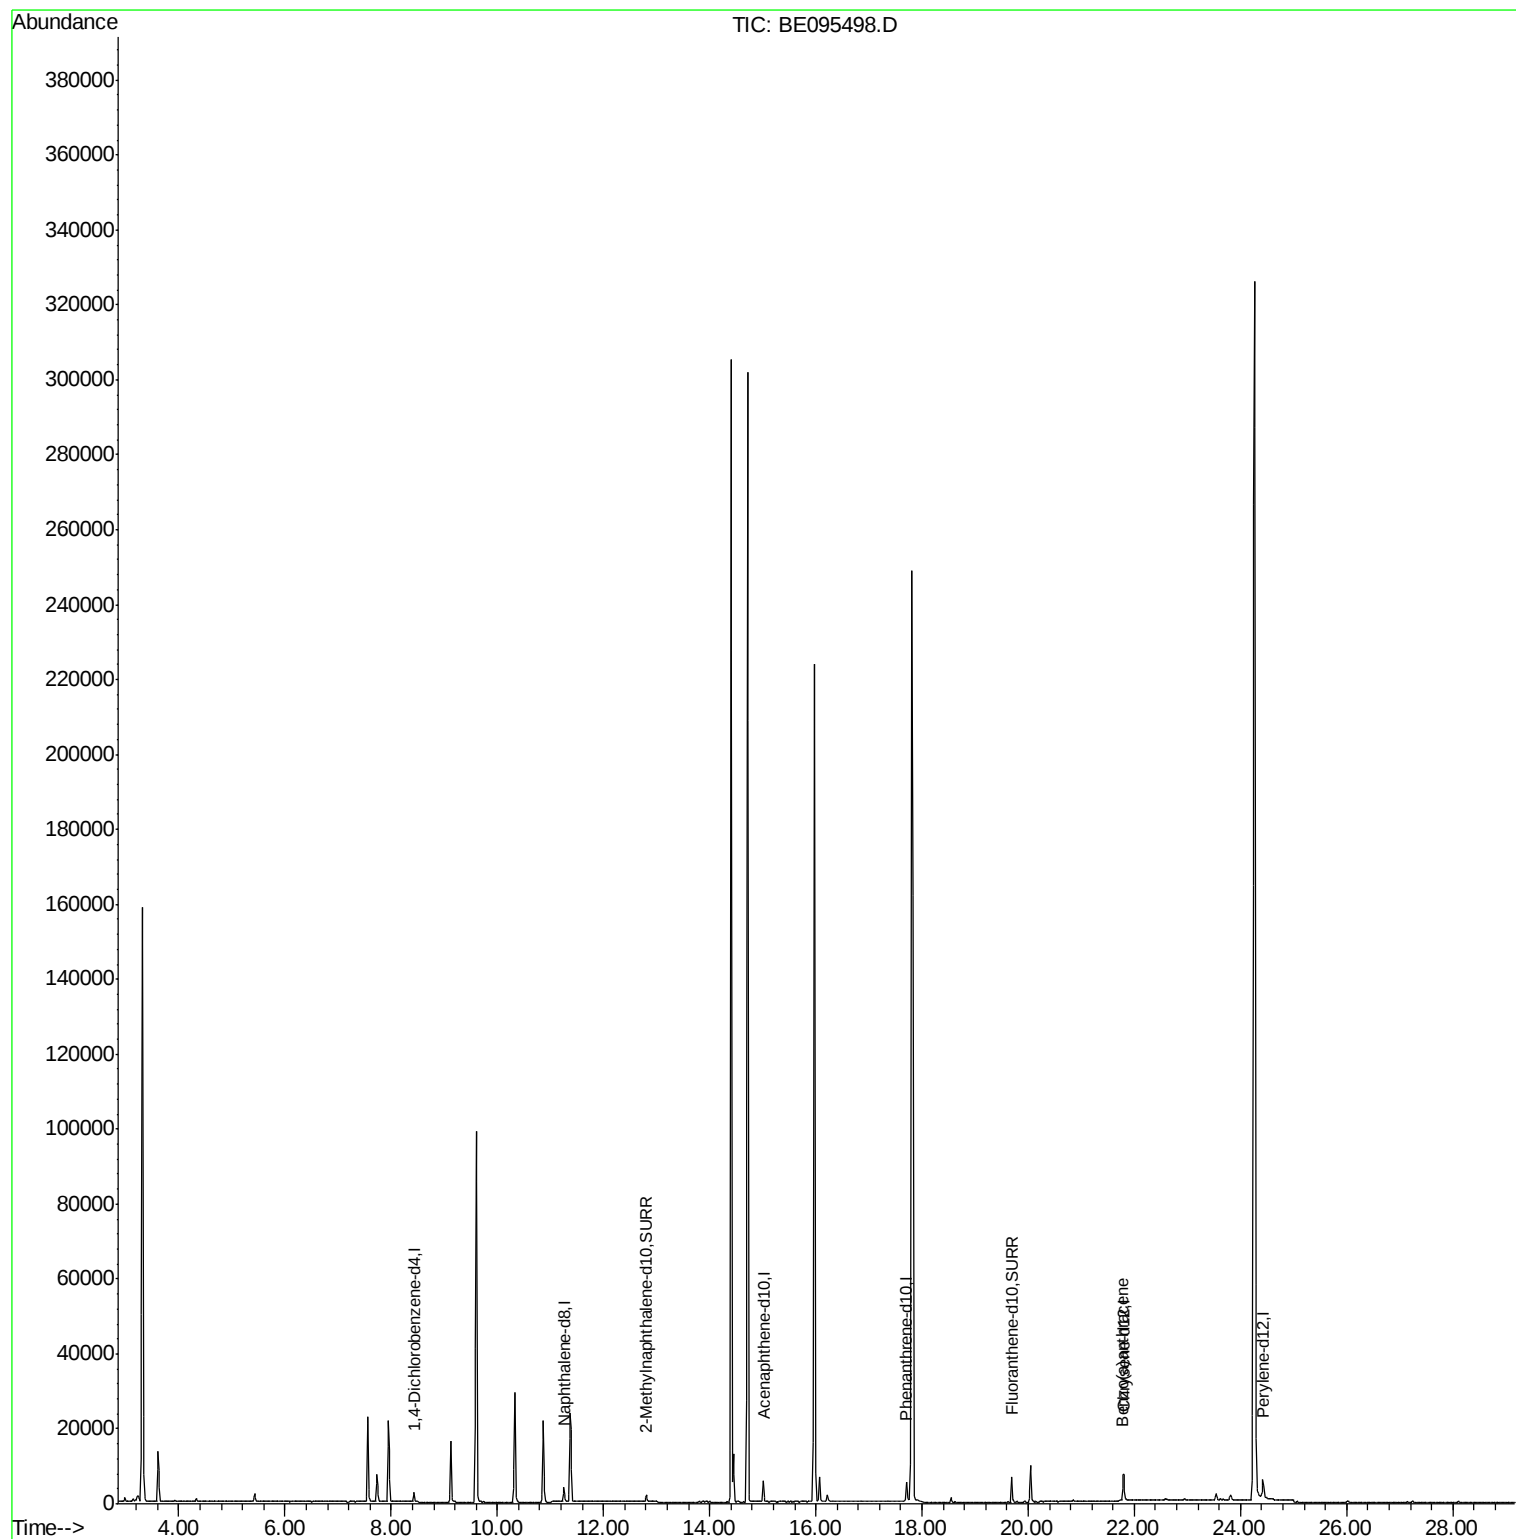

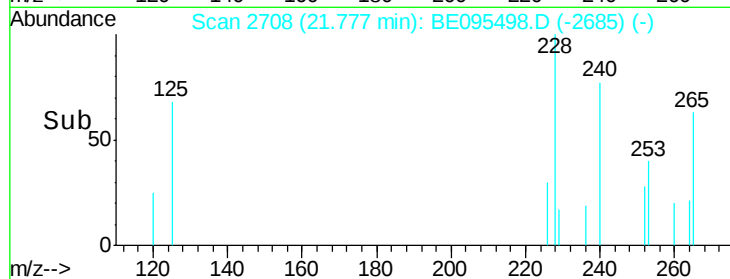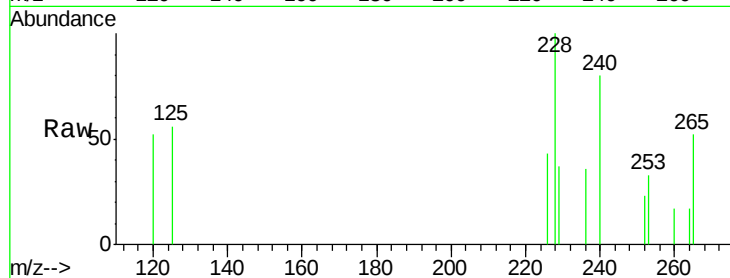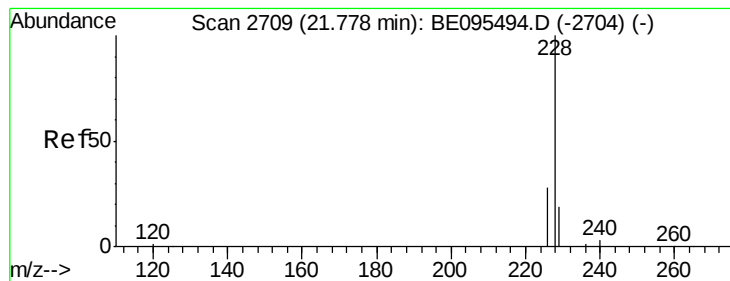

#18

Benzo(a)anthracene

Concen: 0.023 ng/ul

RT: 21.78 min Scan# 2708

Delta R.T. -0.00 min

Lab File: BE095498.D

Acq: 5 Feb 2018 19:37

Instrument :

BNA_E

ClientSampleId :

F6C26

Tgt Ion:228 Resp: 548

Ion Ratio Lower Upper

228 100

229 36.5 22.8 34.2#

226 43.3 17.0 25.6#

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

