

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
 Data File : BE095499.D
 Acq On : 5 Feb 2018 20:10
 Operator : SJ/JU
 Sample : J1296-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C22

Manual Integrations
 APPROVED

Sohil
 2/6/2018 2:30:58 PM

Quant Time: Feb 06 02:58:33 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 02:09:13 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1814	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5067	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3174	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7309	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7444	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	6520m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2792	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7859	0.28	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.30	128	2988	0.211	ng/ul#	90
11) Pentachlorophenol	17.36	266	9305	6.573	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095499.D
Acq On : 5 Feb 2018 20:10
Operator : SJ/JU
Sample : J1296-04
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6C22

Manual Integrations
APPROVED

Sohil
2/6/2018 2:30:58 PM

Quant Time: Feb 06 02:58:33 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration

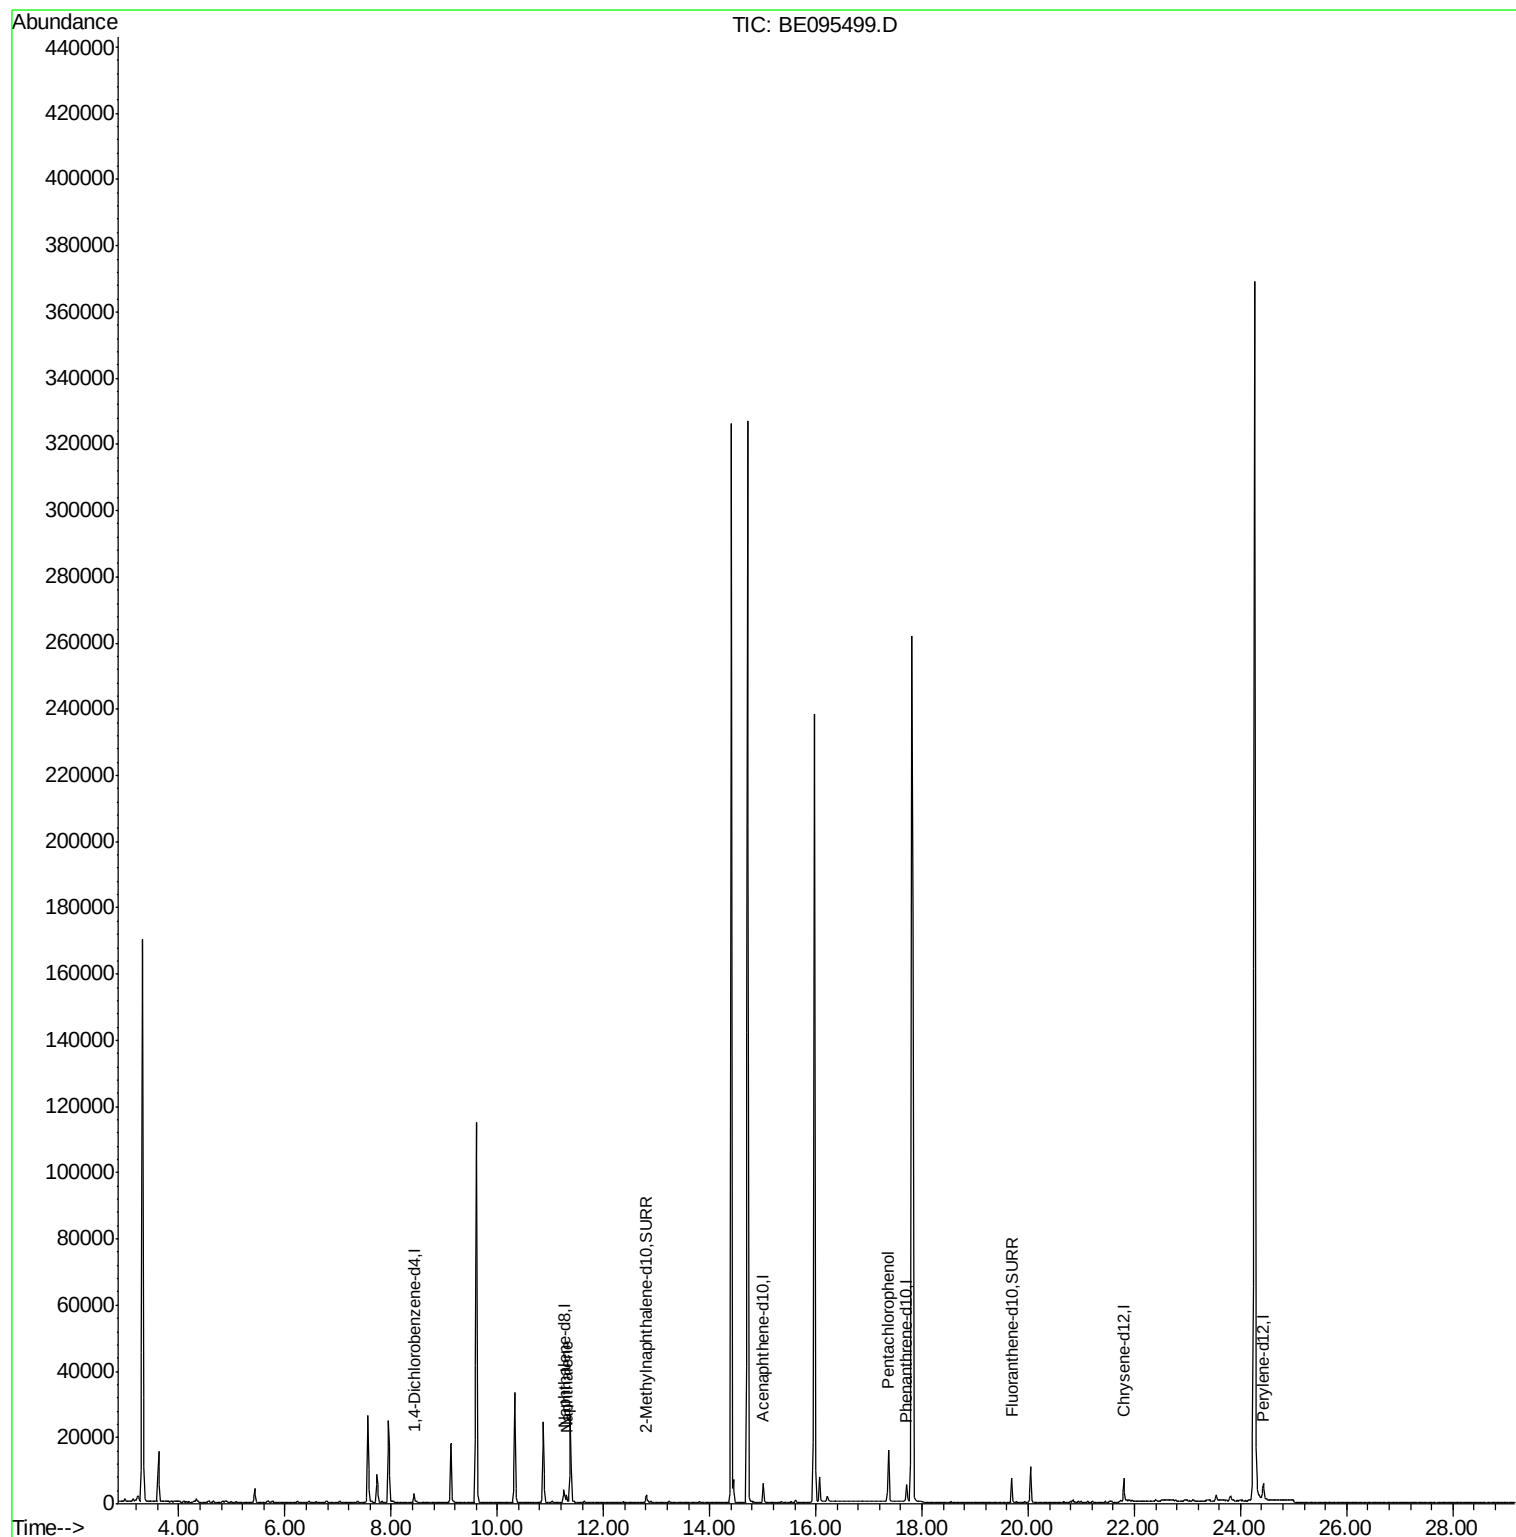

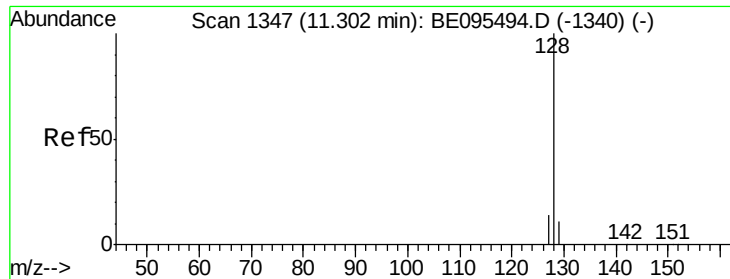

#3

Naphthalene

Concen: 0.211 ng/ul

RT: 11.30 min Scan# 1347

Delta R.T. 0.00 min

Lab File: BE095499.D

Acq: 5 Feb 2018 20:10

Instrument :

BNA_E





ClientSampleId :

F6C22

Tgt Ion:	128	Resp:	2988
Ion Ratio	Lower	Upper	
128	100		
129	13.3	11.3	16.9
127	15.4	4.0	6.0#

Manual Integrations
APPROVED

Sohil
2/6/2018 2:30:58 PM

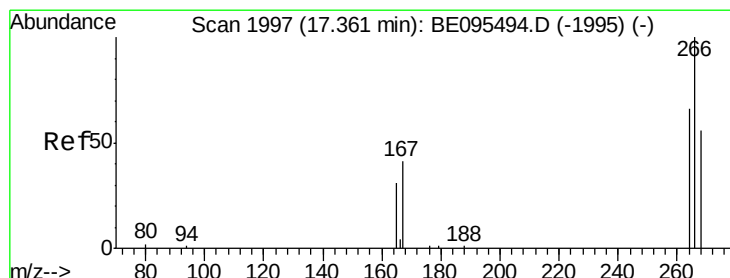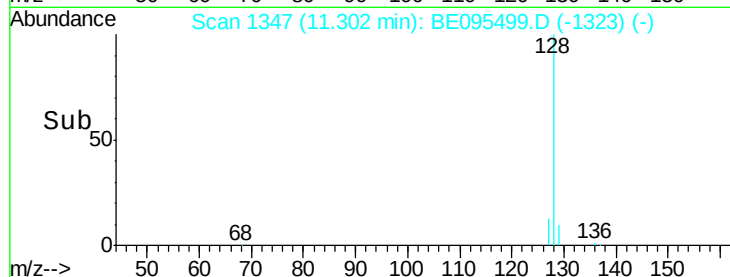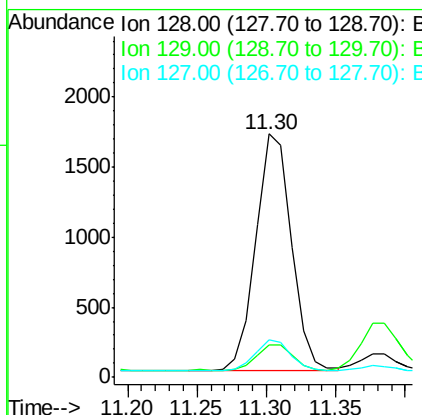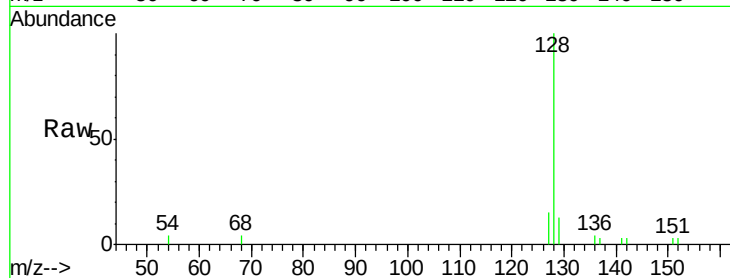

#11

Pentachlorophenol

Concen: 6.573 ng/ul

RT: 17.36 min Scan# 1997

Delta R.T. 0.00 min

Lab File: BE095499.D

Acq: 5 Feb 2018 20:10

Tgt Ion:	266	Resp:	9305
Ion Ratio	Lower	Upper	
266	100		
264	63.4	47.9	71.9
268	62.8	49.8	74.8

