

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
 Data File : BE095509.D
 Acq On : 6 Feb 2018 2:08
 Operator : SJ/JU
 Sample : J1314-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C49

Manual Integrations
 APPROVED

Sohil
 2/6/2018 2:31:34 PM

Quant Time: Feb 06 03:58:55 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 02:09:13 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1784	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5021	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3203	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7396	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7284	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	6766m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2769	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8323	0.29	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	1105	0.771	ng/ul	97
15) Fluoranthene	19.72	202	1221	0.038	ng/ul	86
17) Pyrene	20.08	202	935	0.038	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020518\
Data File : BE095509.D
Acq On : 6 Feb 2018 2:08
Operator : SJ/JU
Sample : J1314-12
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6C49

Manual Integrations
APPROVED

Sohil
2/6/2018 2:31:34 PM

Quant Time: Feb 06 03:58:55 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 02:09:13 2018
Response via : Initial Calibration

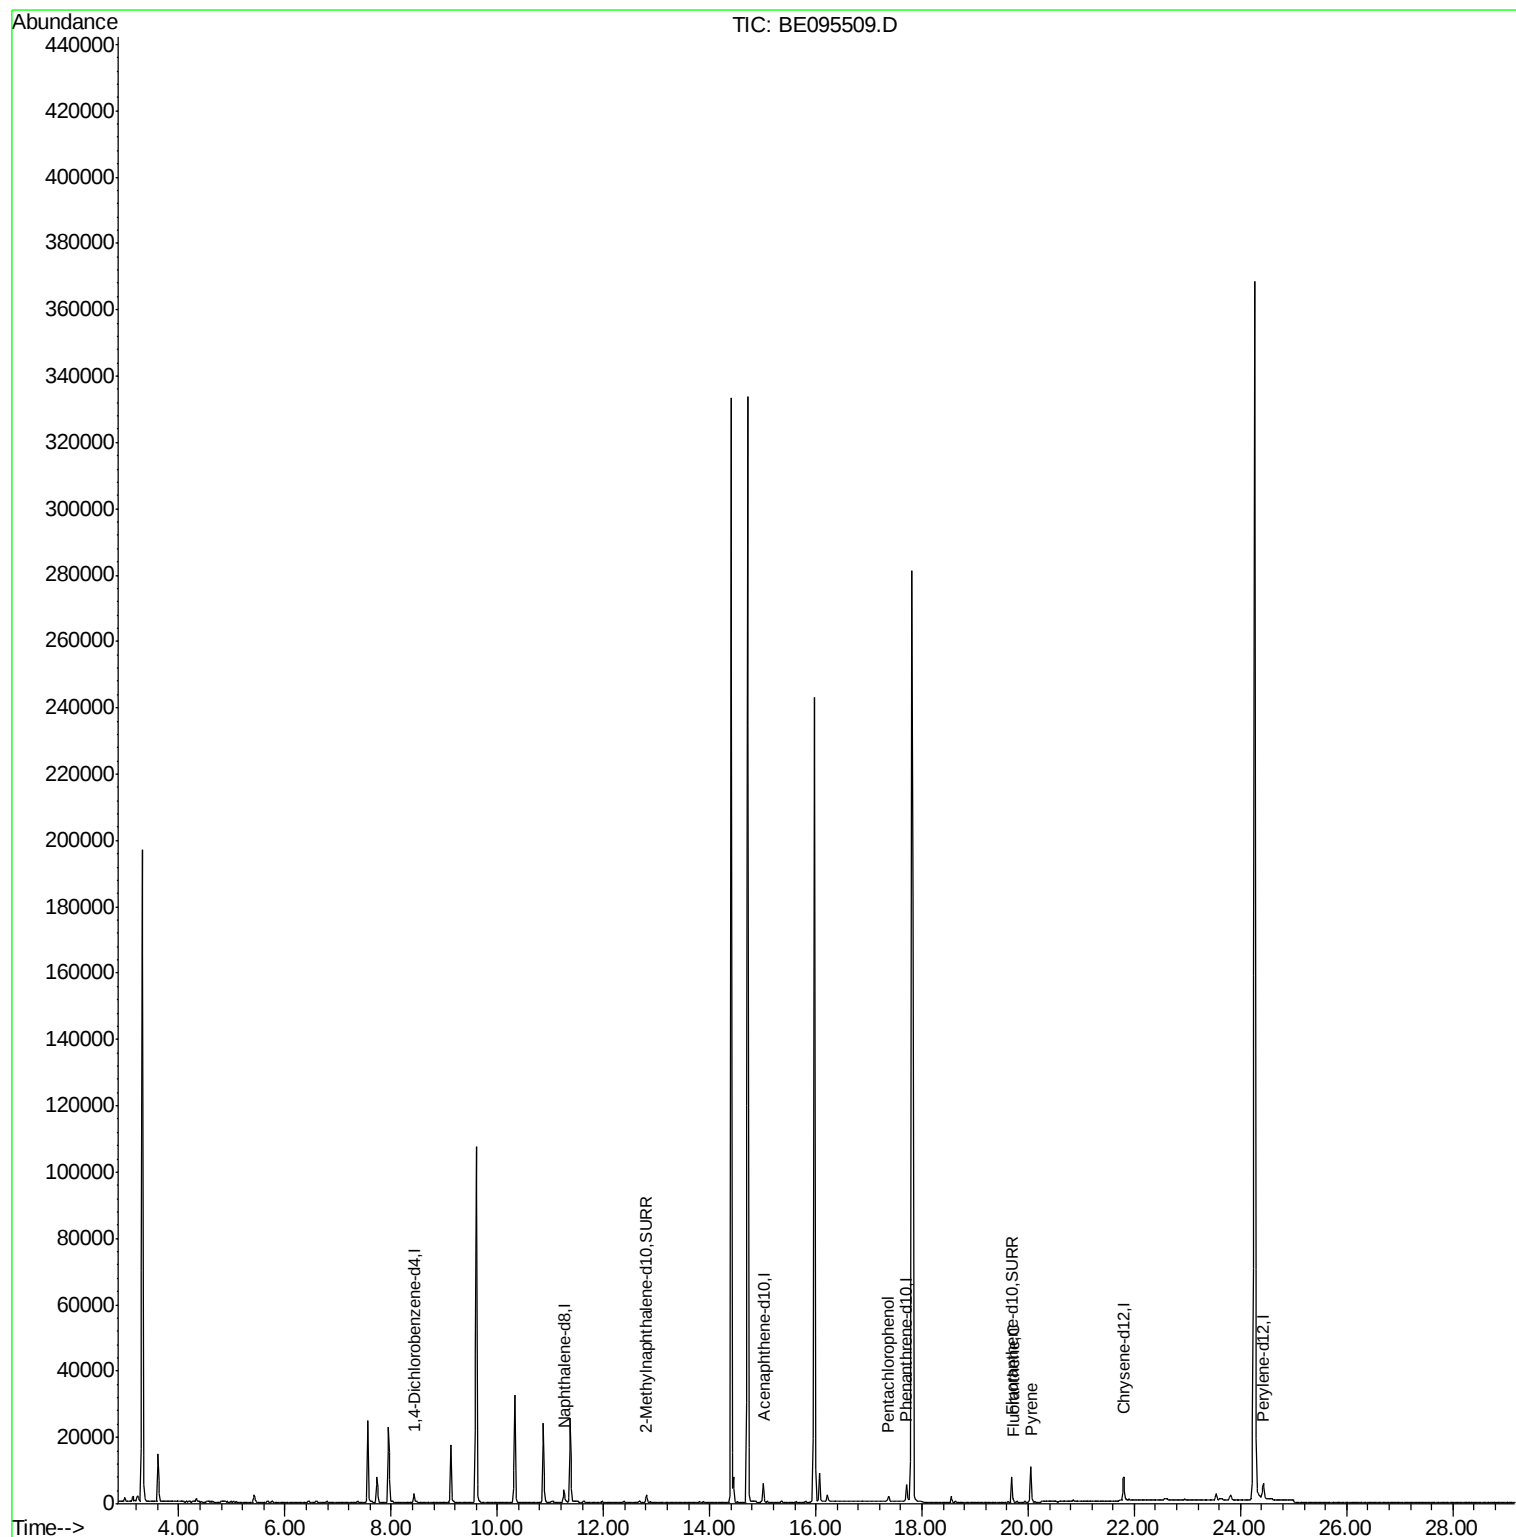

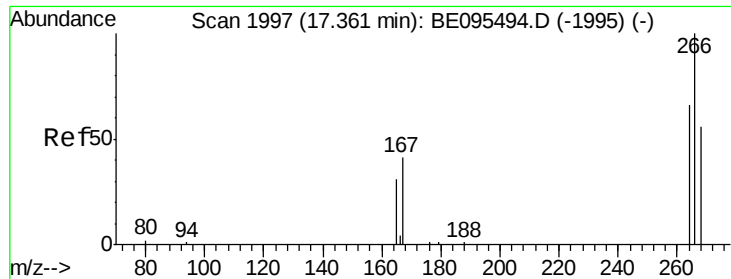





#11
 Pentachlorophenol
 Concen: 0.771 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095509.D
 Acq: 6 Feb 2018 2:08

Instrument :
 BNA_E
 ClientSampleId :
 F6C49

Tgt Ion	Ratio	Lower	Upper
266	100		
264	63.3	47.9	71.9
268	62.9	49.8	74.8




Manual Integrations
 APPROVED




Sohil
 2/6/2018 2:31:34 PM

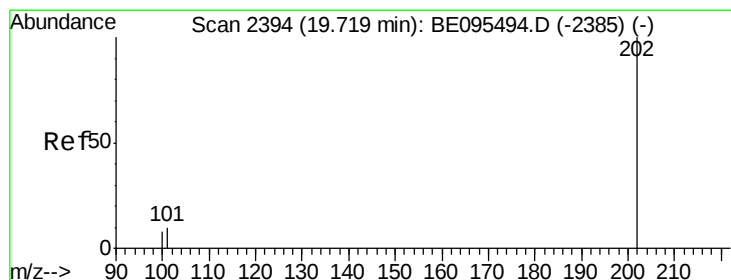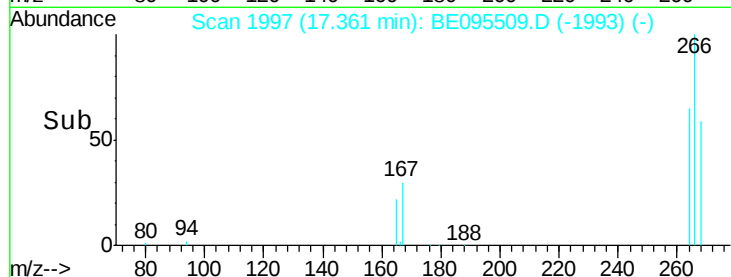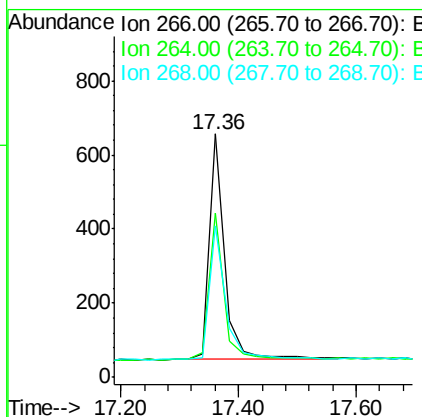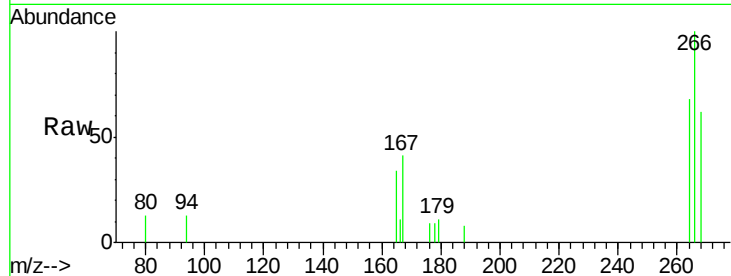

#15
 Fluoranthene
 Concen: 0.038 ng/ul
 RT: 19.72 min Scan# 2394
 Delta R.T. 0.00 min
 Lab File: BE095509.D
 Acq: 6 Feb 2018 2:08

Tgt Ion	Ratio	Lower	Upper
202	100		
101	15.9	0.0	30.3
100	13.4	0.0	39.5

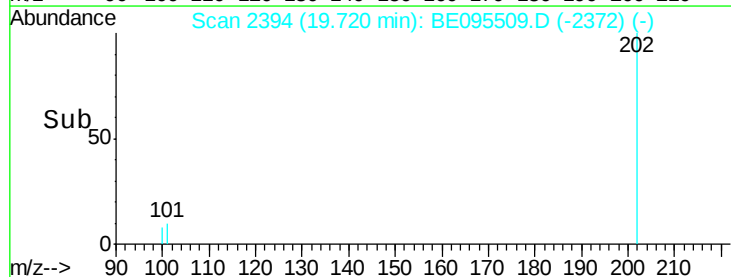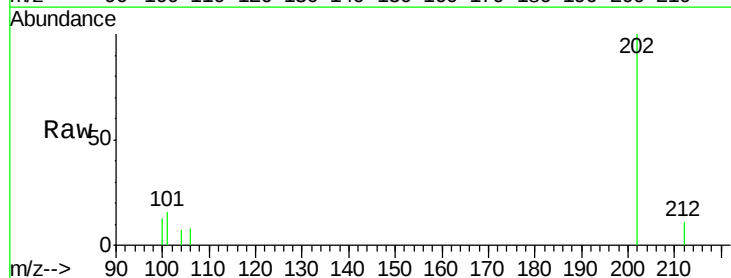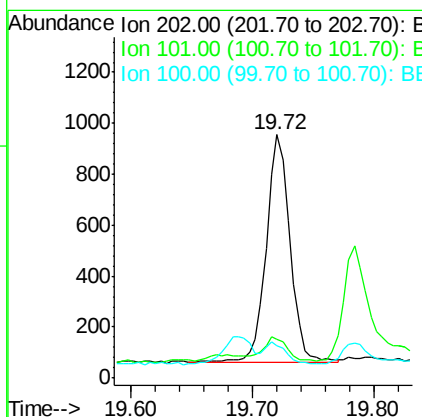

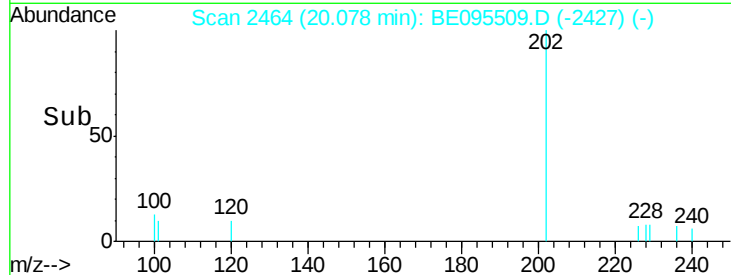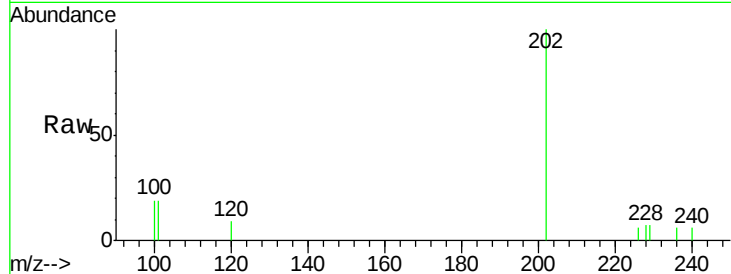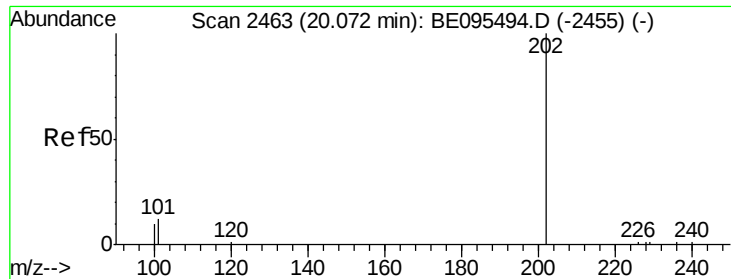

#17
 Pyrene
 Concen: 0.038 ng/ul
 RT: 20.08 min Scan# 2464
 Delta R.T. 0.01 min
 Lab File: BE095509.D
 Acq: 6 Feb 2018 2:08

Instrument :
 BNA_E
 ClientSampleId :
 F6C49

Tgt Ion:	202	Resp:	935
Ion Ratio	Lower	Upper	
202	100		
101	18.9	18.2	27.4
100	18.6	15.6	23.4

Manual Integrations
 APPROVED

Sohil
 2/6/2018 2:31:34 PM

