


Data Path : Z:\HPCHEM1\BNA_M\Data\BM020615\
 Data File : BM000441.D
 Acq On : 06 Feb 2015 19:30
 Operator : TP/IZ
 Sample : DFTPP19
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP19

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM020615.M
 Title : SVOA CALIBRATION
 Last Update : Sat Feb 07 02:55:14 2015

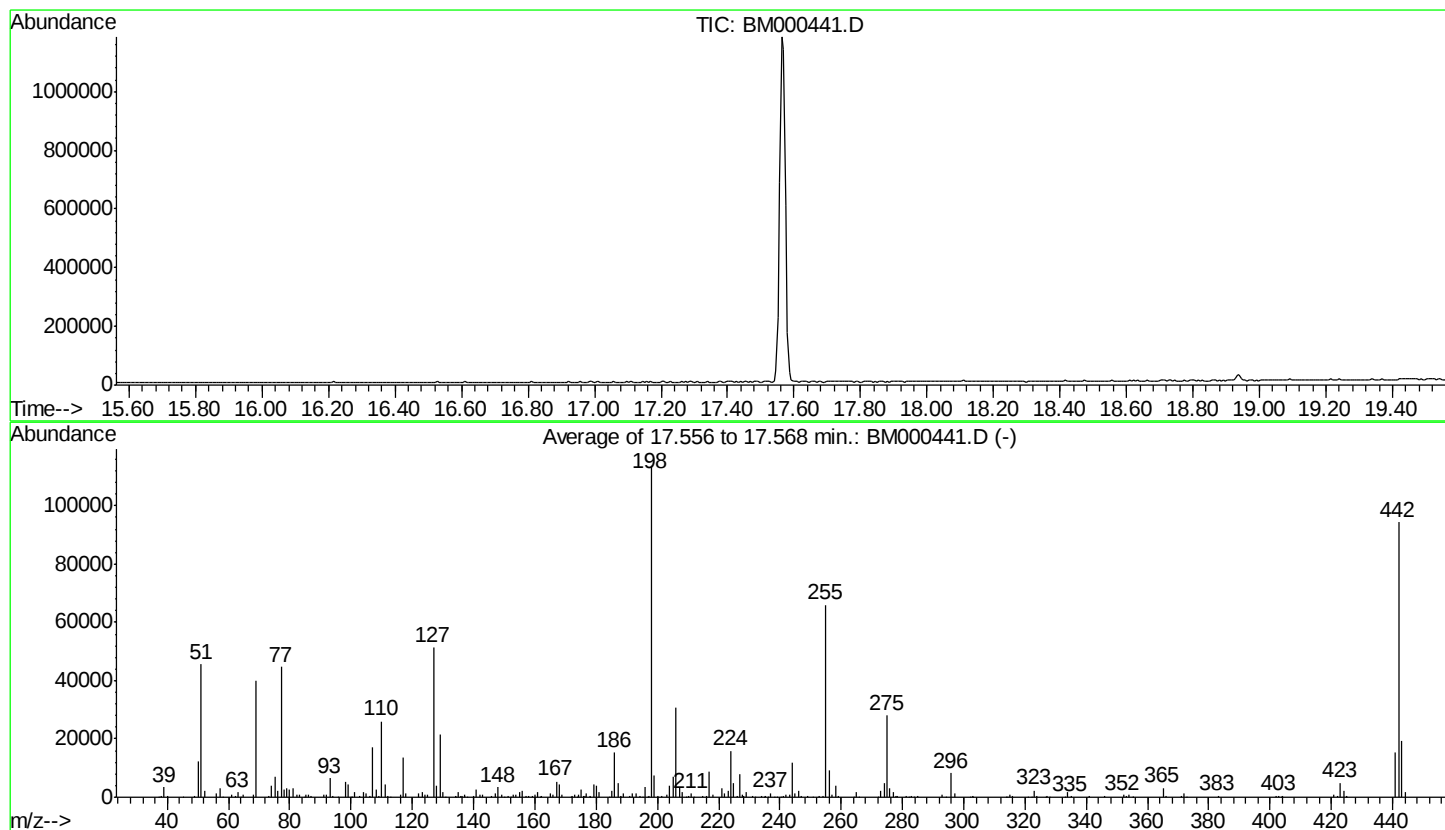

AutoFind: Scans 2528, 2529, 2530; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	45488	PASS
68	69	0.00	2	1.9	751	PASS
69	198	0.00	100	35.0	39850	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.0	51184	PASS
197	198	0.00	2	0.5	530	PASS
198	198	100	100	100.0	113765	PASS
199	198	5	9	6.7	7603	PASS
275	198	10	60	24.6	28018	PASS
365	198	1	100	2.8	3216	PASS
441	443	0.01	100	78.5	15259	PASS
442	198	50	100	82.9	94269	PASS
443	442	15	24	20.6	19442	PASS