


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE020615\
 Data File : BE089523.D
 Acq On : 6 Feb 2015 11:11
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE020615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 07 04:07:57 2015

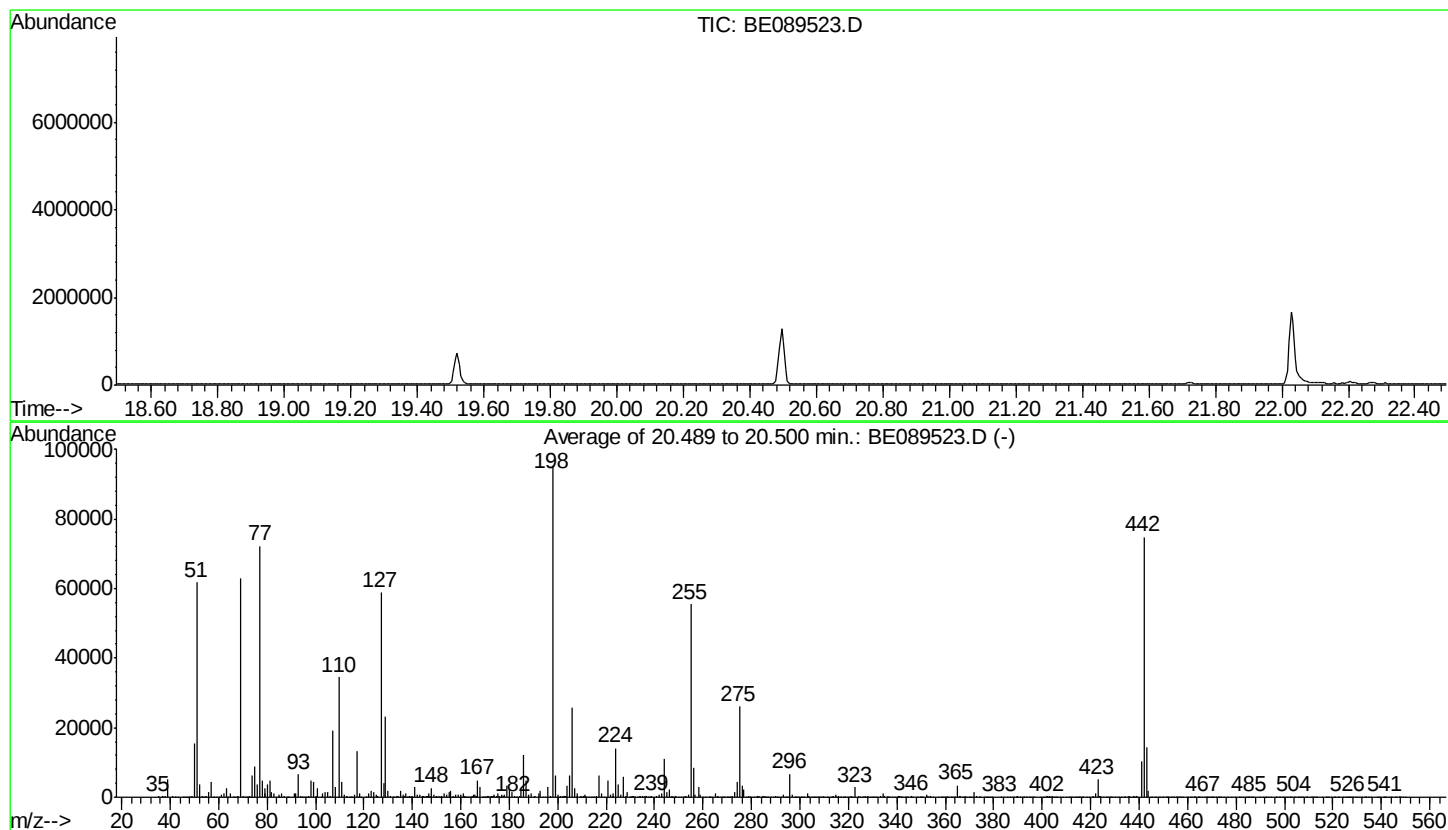

AutoFind: Scans 3251, 3252, 3253; Background Corrected with Scan 3244

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.7	61632	PASS
68	69	0.00	2	0.7	457	PASS
69	198	0.00	100	66.2	63082	PASS
70	69	0.00	2	0.5	302	PASS
127	198	10	80	61.6	58692	PASS
197	198	0.00	2	0.4	356	PASS
198	198	100	100	100.0	95273	PASS
199	198	5	9	6.5	6232	PASS
275	198	10	60	27.2	25940	PASS
365	198	1	100	3.5	3318	PASS
441	442	0.01	24	13.9	10357	PASS
442	198	50	100	78.4	74668	PASS
443	442	15	24	19.3	14433	PASS