


Data Path : Z:\HPCHEM1\BNA_E\Data\BE020615\
 Data File : BE089540.D
 Acq On : 6 Feb 2015 23:40
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE020615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 07 04:07:57 2015

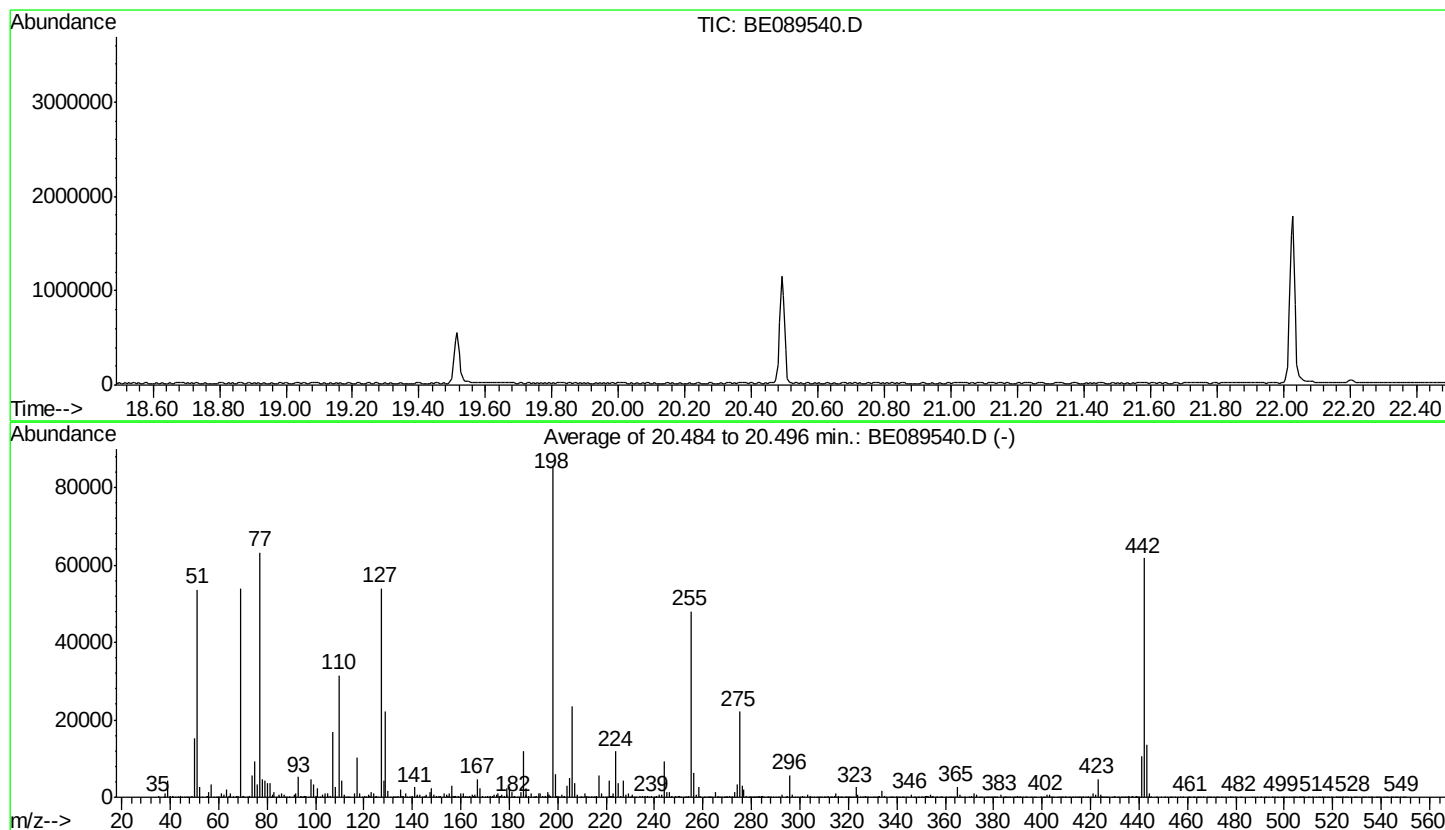

AutoFind: Scans 3250, 3251, 3252; Background Corrected with Scan 3242

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.6	53602	PASS
68	69	0.00	2	0.9	464	PASS
69	198	0.00	100	62.9	53839	PASS
70	69	0.00	2	0.8	412	PASS
127	198	10	80	62.9	53888	PASS
197	198	0.00	2	0.3	228	PASS
198	198	100	100	100.0	85639	PASS
199	198	5	9	6.8	5819	PASS
275	198	10	60	25.8	22129	PASS
365	198	1	100	3.1	2674	PASS
441	442	0.01	24	17.0	10473	PASS
442	198	50	100	72.1	61776	PASS
443	442	15	24	21.7	13427	PASS