
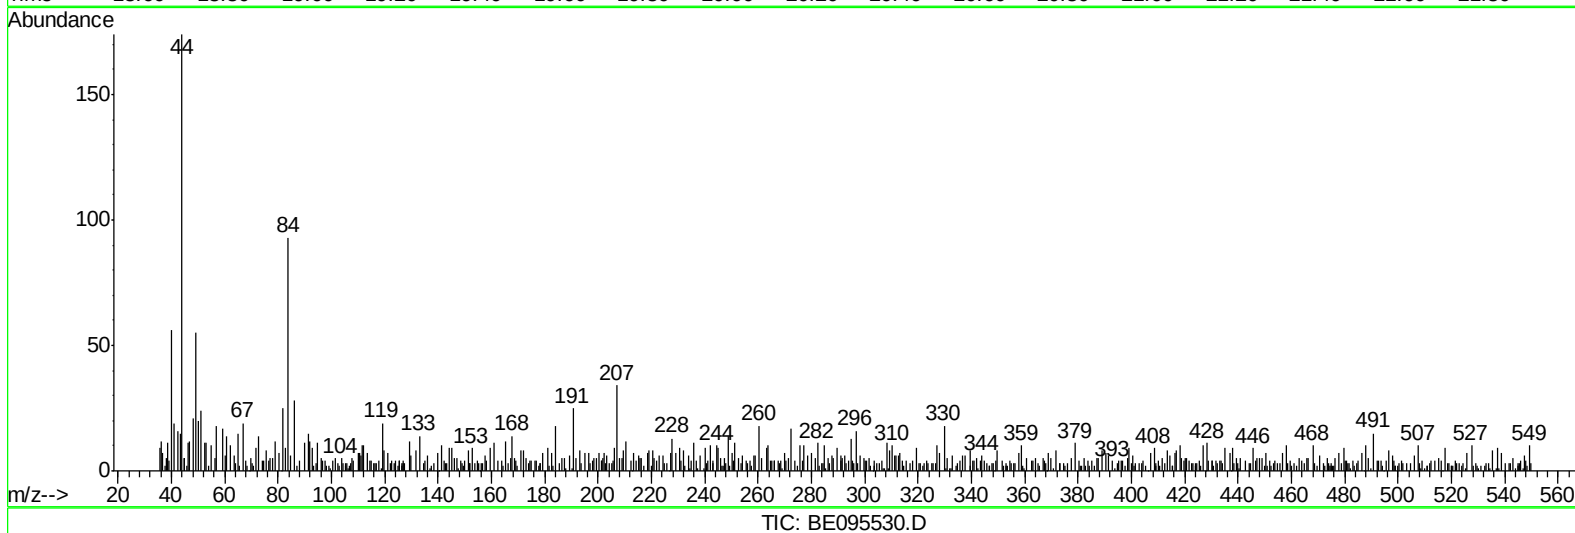


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020618\
Data File : BE095530.D
Acq On : 6 Feb 2018 15:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 06:01:09 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

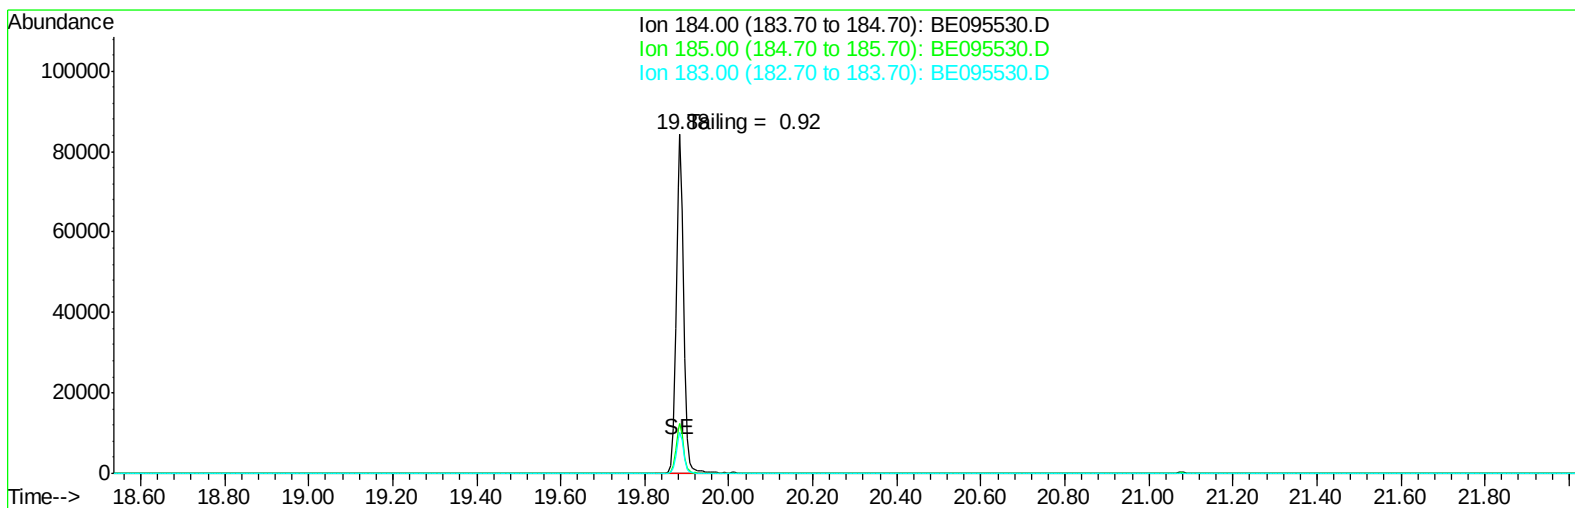

(76) Benzidine



12.716min (-0.023) 78.33ng

response 18

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.67
183.00	11.60	11.11
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020618\
Data File : BE095530.D
Acq On : 6 Feb 2018 15:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 06:01:09 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

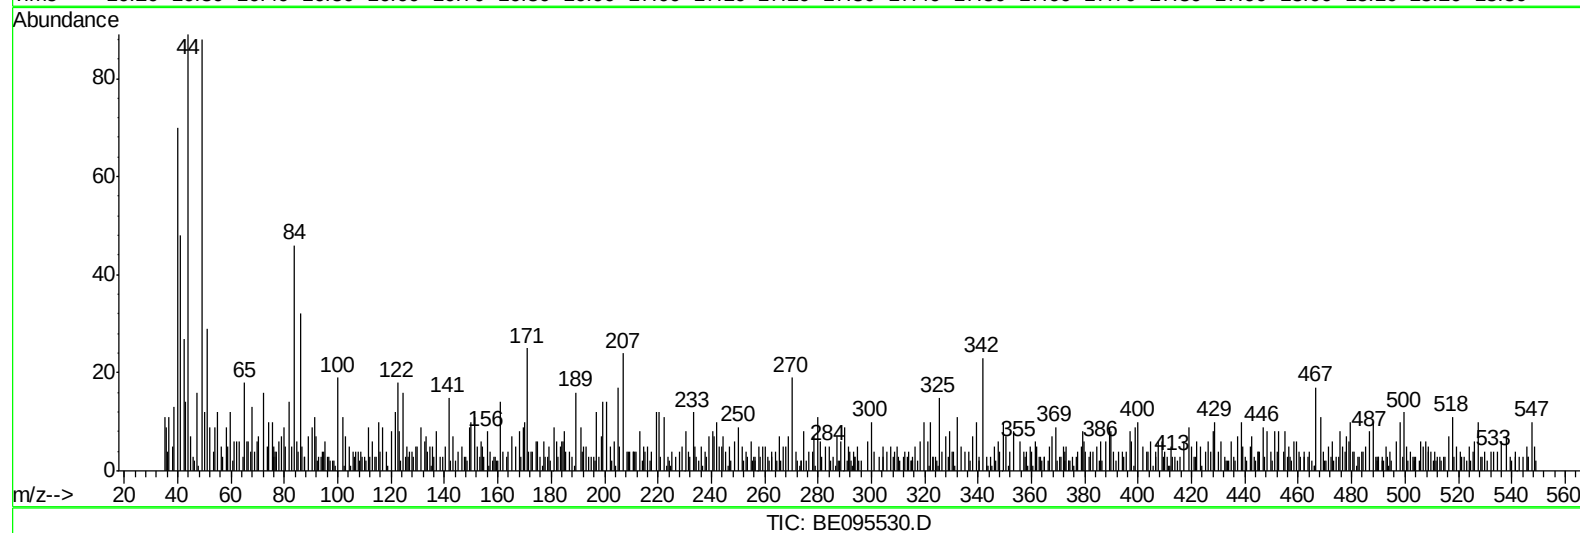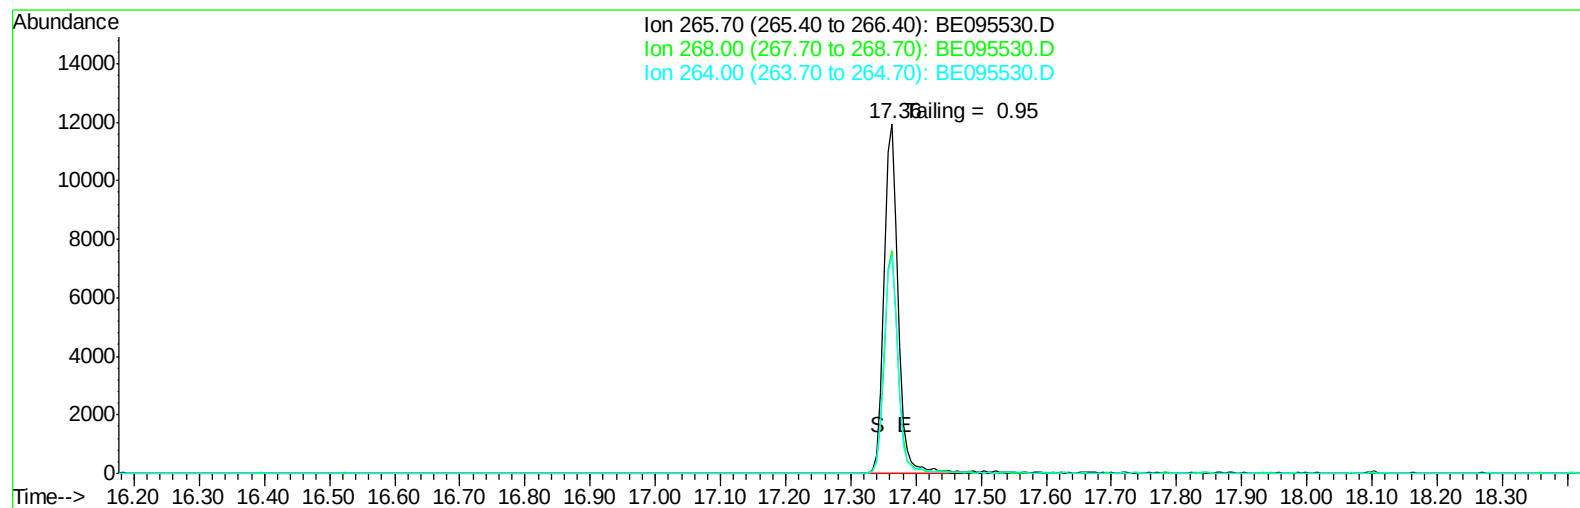

(69) Pentachlorophenol (C)

11.053min (-0.156) 170.31ng

response 7

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	55.56
264.00	61.90	66.67
0.00	0.00	0.00