


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020618\
 Data File : BE095530.D
 Acq On : 6 Feb 2018 15:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 06 20:27:34 2018

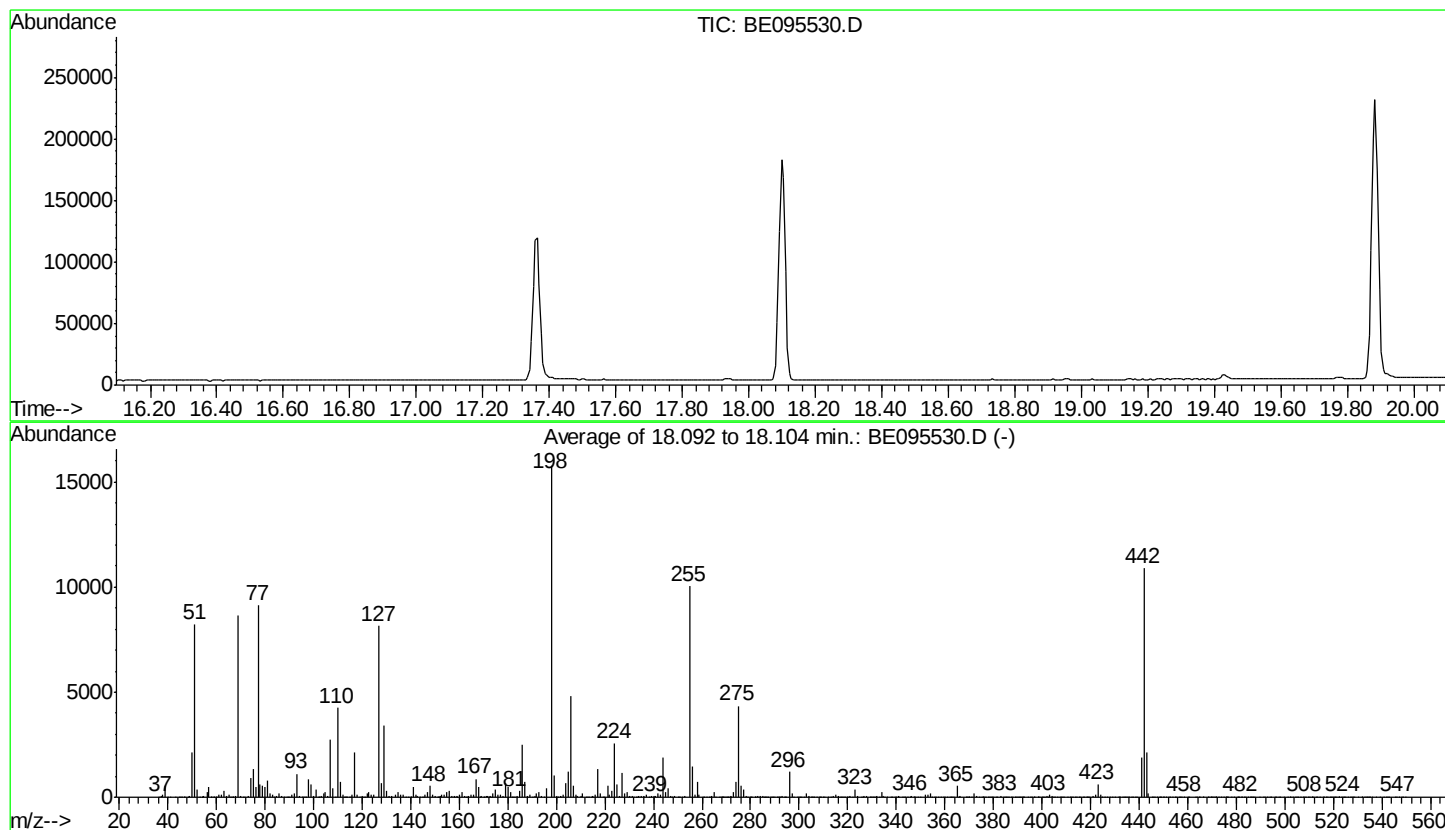

AutoFind: Scans 2639, 2640, 2641; Background Corrected with Scan 2630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.0	8207	PASS
68	69	0.00	2	0.5	43	PASS
69	198	0.00	100	54.7	8635	PASS
70	69	0.00	2	0.5	43	PASS
127	198	10	80	51.6	8143	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15781	PASS
199	198	5	9	6.4	1011	PASS
275	198	10	60	27.5	4332	PASS
365	198	1	100	3.4	540	PASS
441	442	0.01	24	17.1	1861	PASS
442	198	50	100	68.9	10876	PASS
443	442	15	24	19.6	2135	PASS