
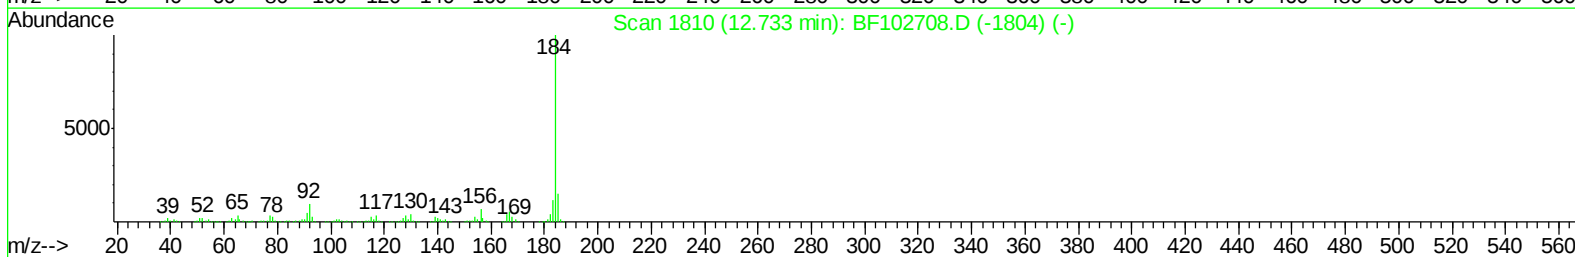
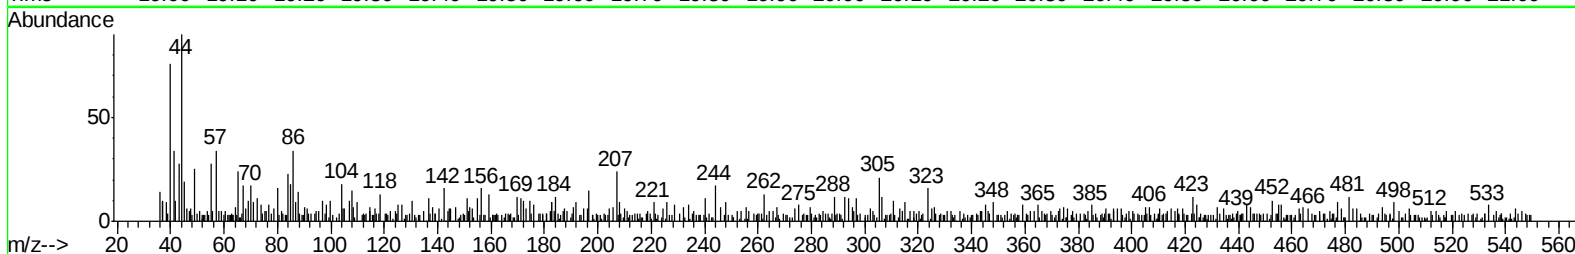


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020718\
Data File : BE095544.D
Acq On : 7 Feb 2018 8:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 03:14:42 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

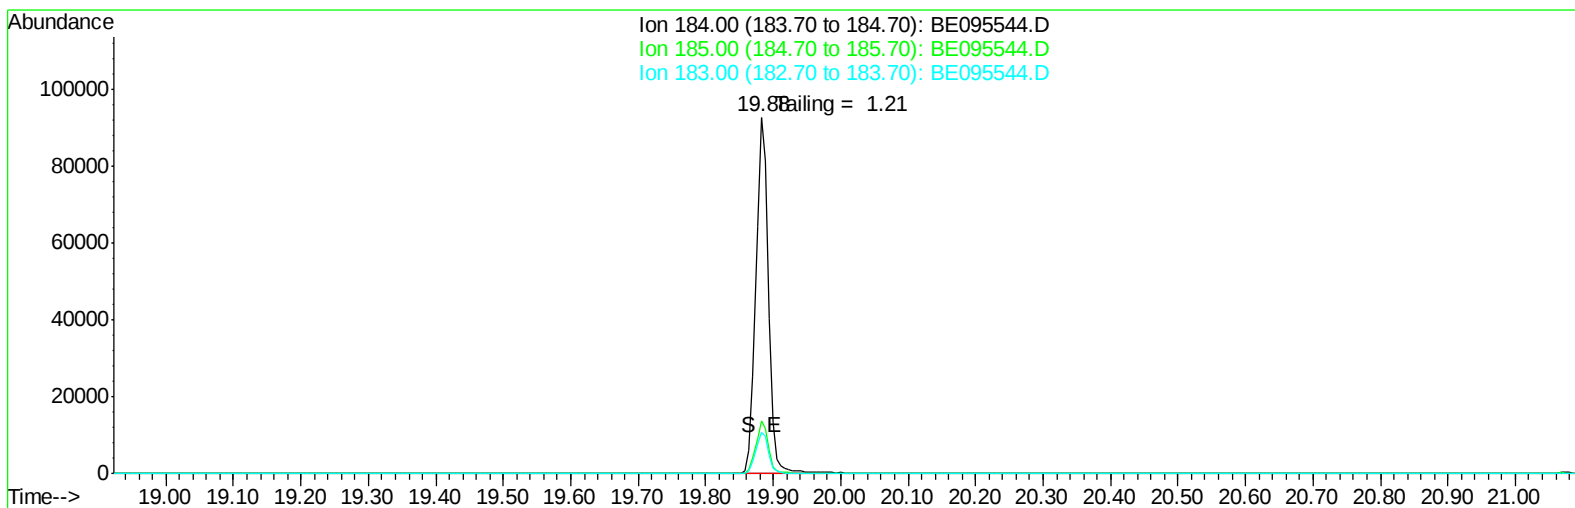

TIC: BE095544.D

(76) Benzidine




13.119min (+0.380) 23.93ng

response 11

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	41.67#
183.00	11.60	116.67#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020718\
Data File : BE095544.D
Acq On : 7 Feb 2018 8:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 03:14:42 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

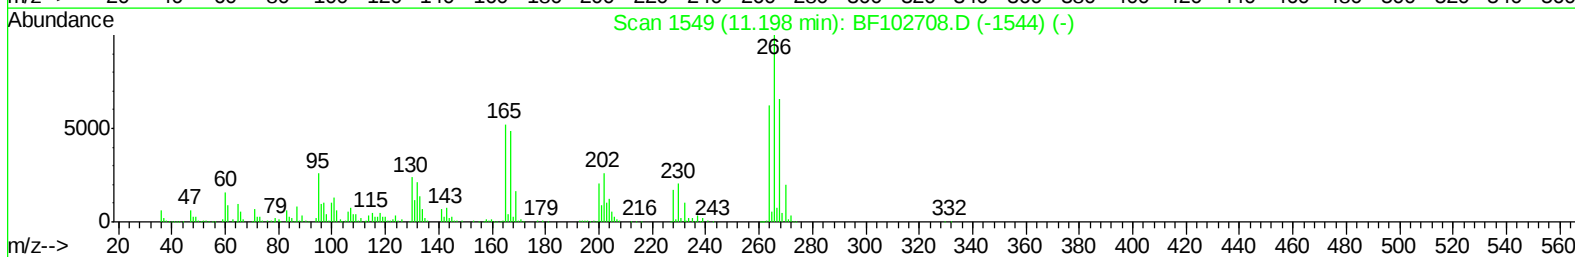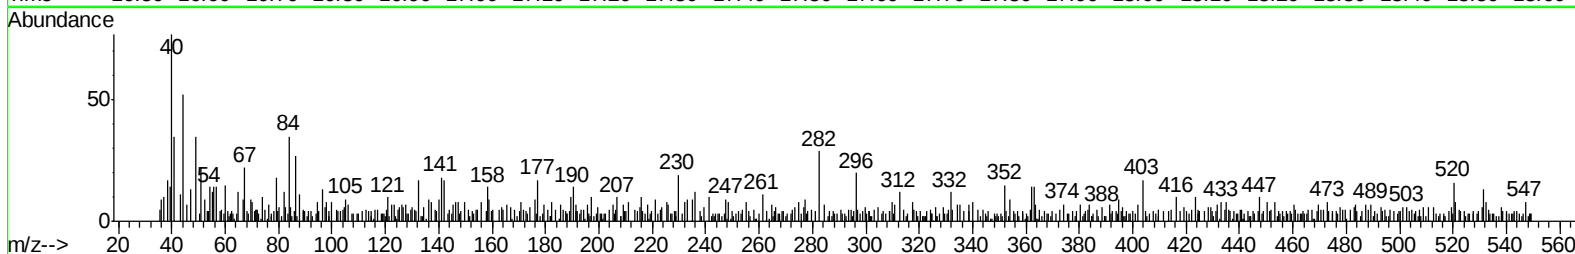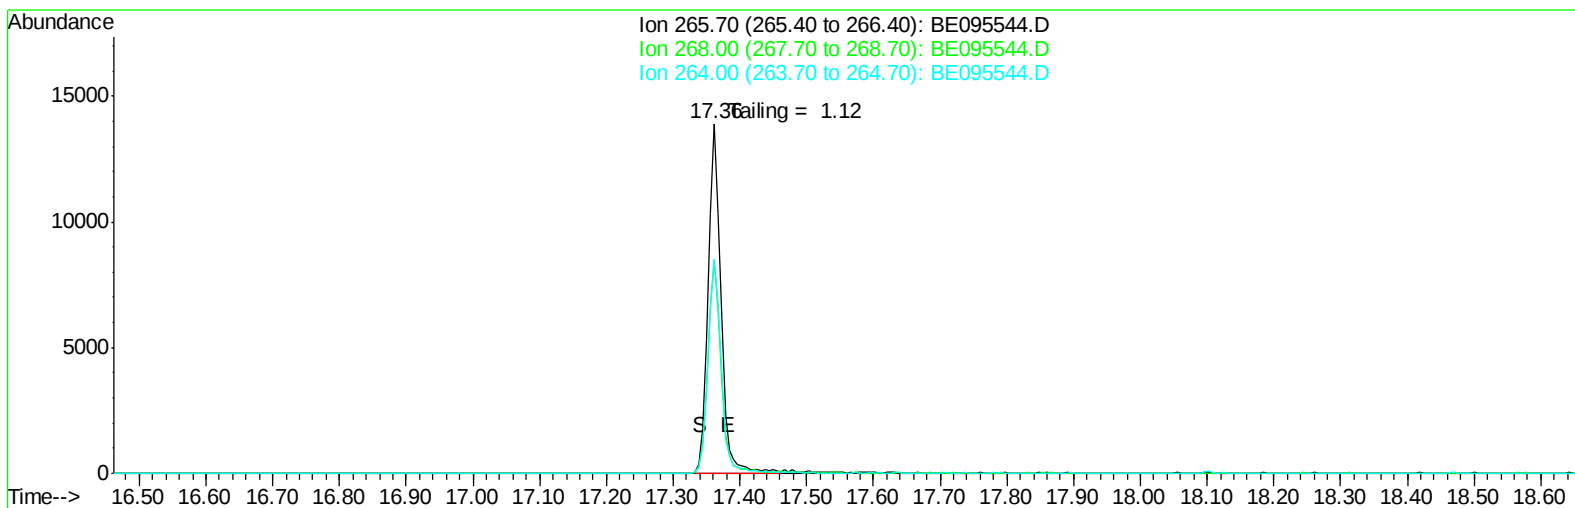

TIC: BE095544.D

(69) Pentachlorophenol (C)

11.680min (+0.470) 291.96ng

response 10

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	70.00
264.00	61.90	70.00
0.00	0.00	0.00