


Data Path : Z:\HPCHEM1\BNA_E\Data\BE020718\
 Data File : BE095544.D
 Acq On : 7 Feb 2018 8:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 17 02:59:40 2018

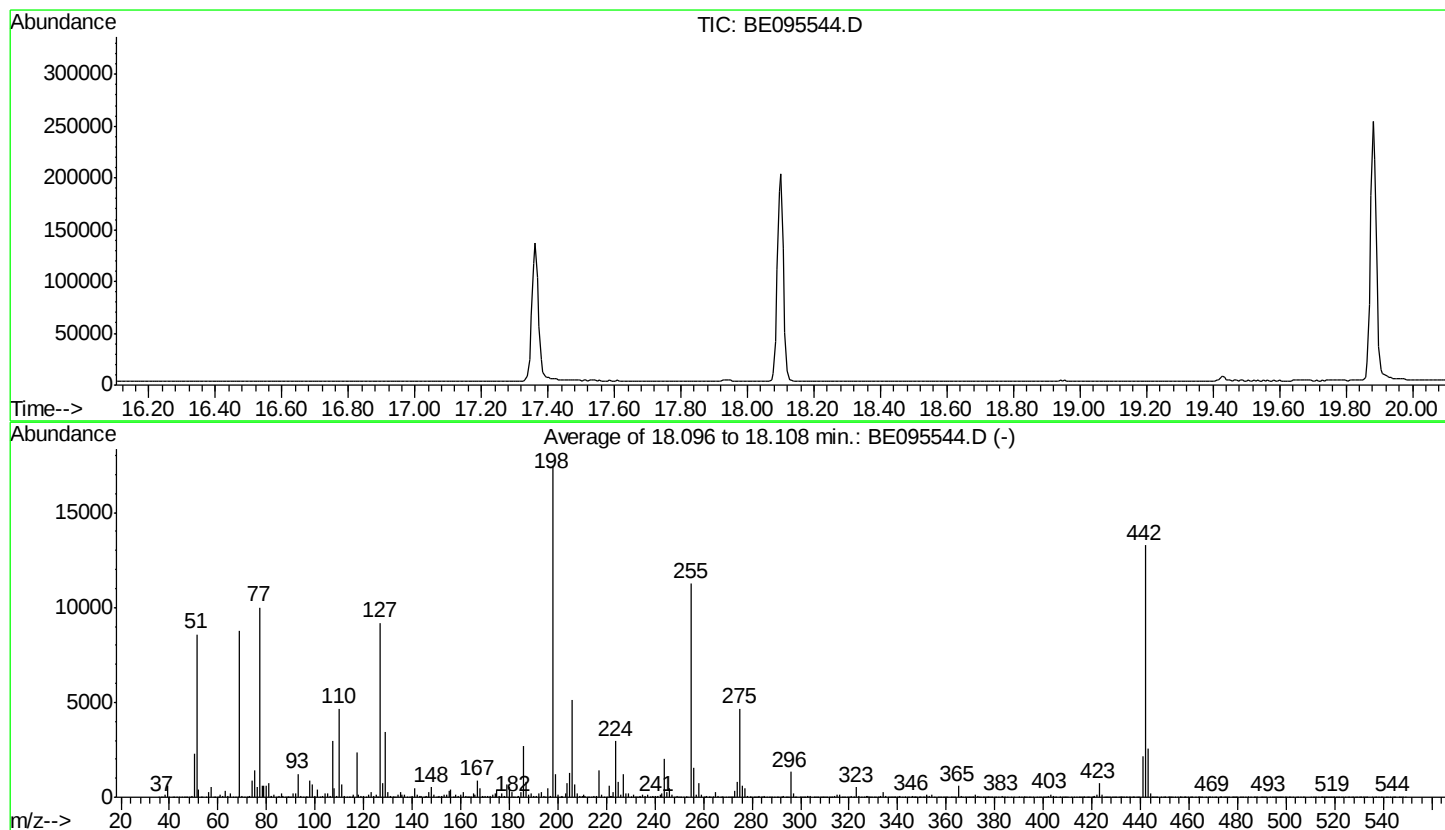

AutoFind: Scans 2639, 2640, 2641; Background Corrected with Scan 2630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.0	8565	PASS
68	69	0.00	2	0.2	21	PASS
69	198	0.00	100	50.4	8801	PASS
70	69	0.00	2	0.5	41	PASS
127	198	10	80	52.7	9202	PASS
197	198	0.00	2	0.3	47	PASS
198	198	100	100	100.0	17467	PASS
199	198	5	9	7.0	1230	PASS
275	198	10	60	26.7	4669	PASS
365	198	1	100	3.4	598	PASS
441	442	0.01	24	16.0	2128	PASS
442	198	50	100	76.0	13281	PASS
443	442	15	24	19.2	2554	PASS