

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
 Data File : BE095569.D
 Acq On : 8 Feb 2018 15:07
 Operator : SJ/JU
 Sample : J1316-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 09 00:47:40 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 09 00:43:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1637	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4395	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3038	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6514	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6575	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	500652	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3169	0.44	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9057	0.36	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	43	0.034	ng/ul	86
17) Pyrene	20.05	202	1716	0.078	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
Data File : BE095569.D
Acq On : 8 Feb 2018 15:07
Operator : SJ/JU
Sample : J1316-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 09 00:47:40 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 00:43:28 2018
Response via : Initial Calibration




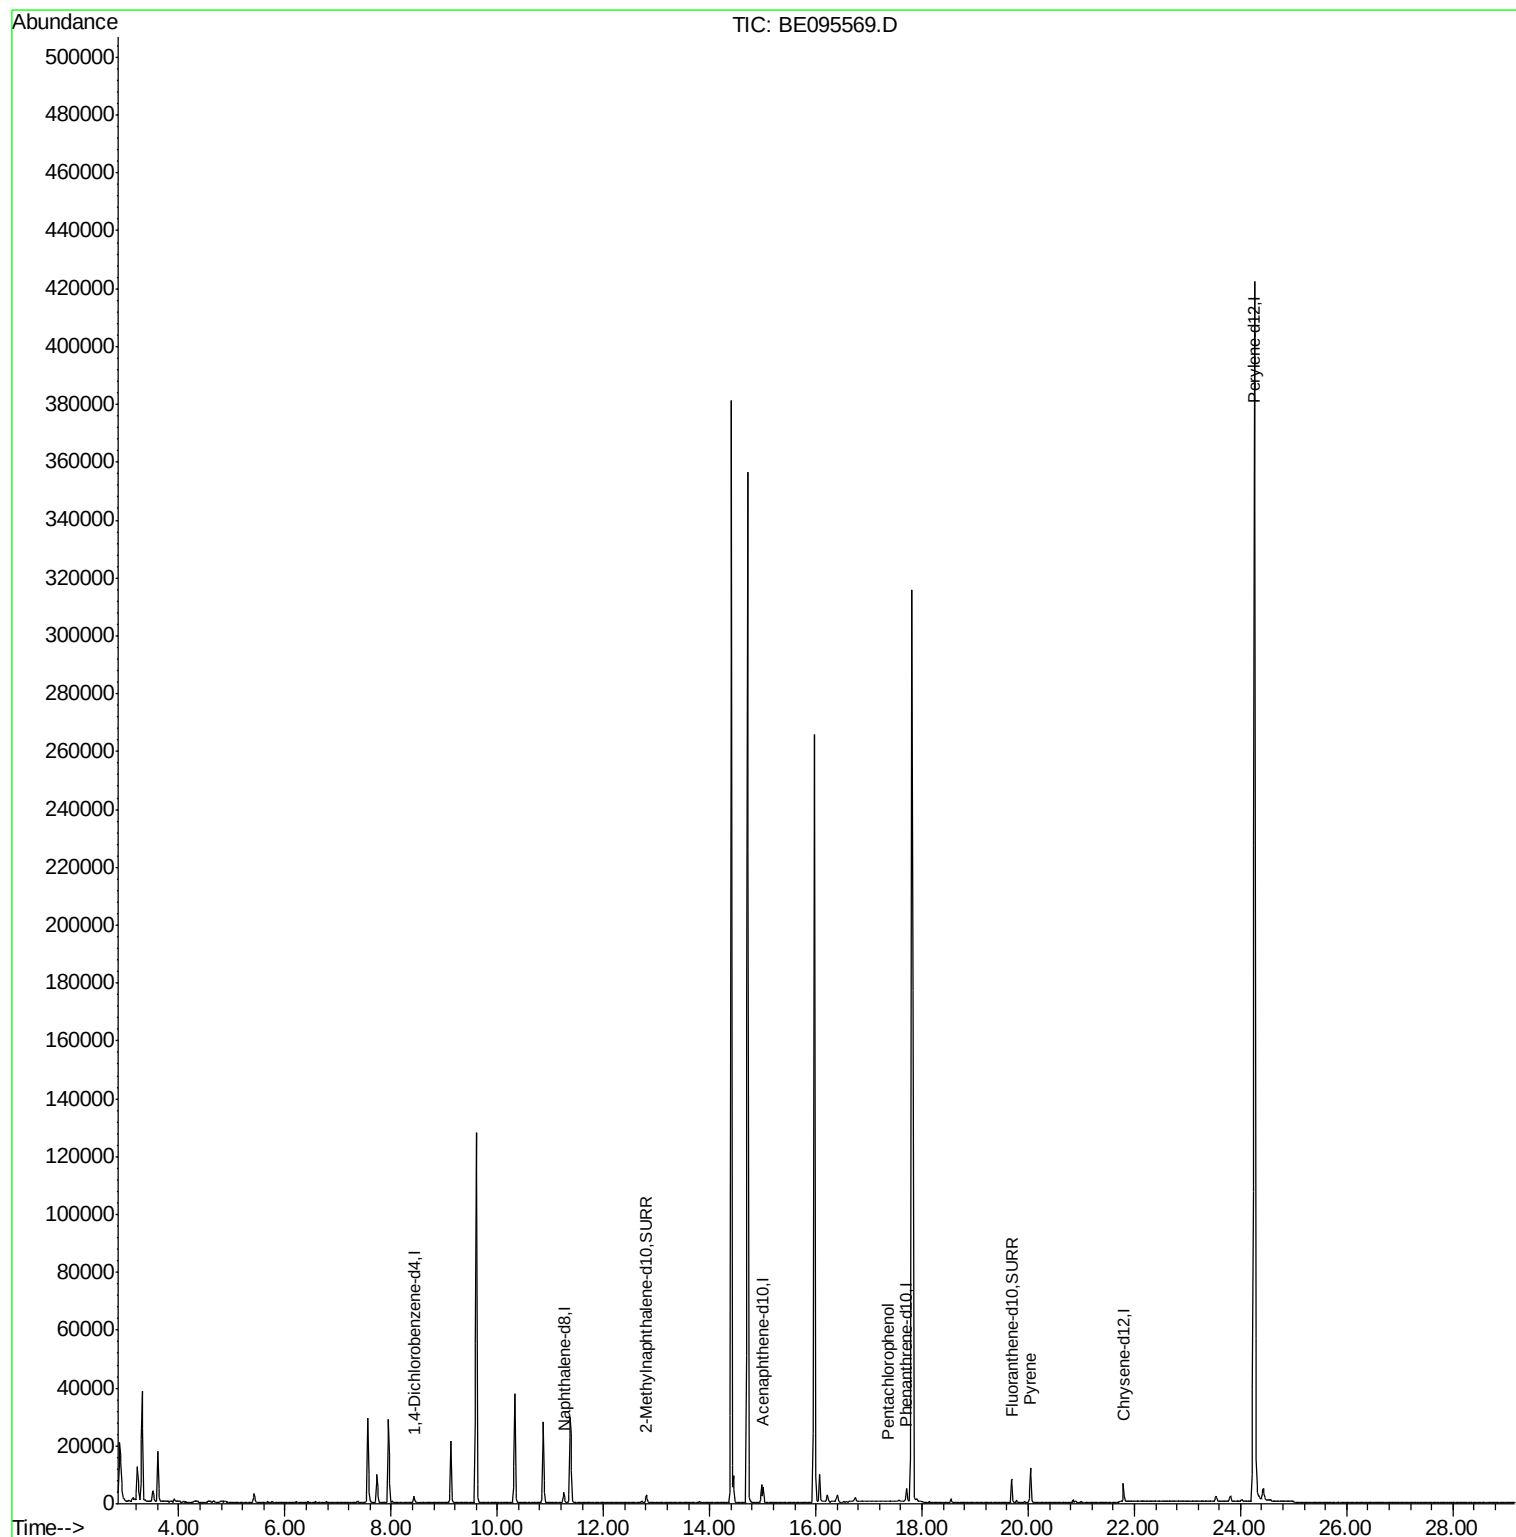


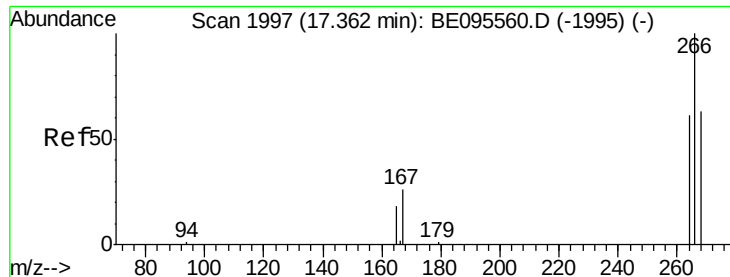

#11
 Pentachlorophenol
 Concen: 0.034 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095569.D
 Acq: 8 Feb 2018 15:07

Instrument :
 BNA_E
 ClientSampled :

Tot Ion:266 Resp: 43
 Ion Ratio Lower Upper
 266 100
 264 51.2 47.9 71.9
 268 74.4 49.8 74.8

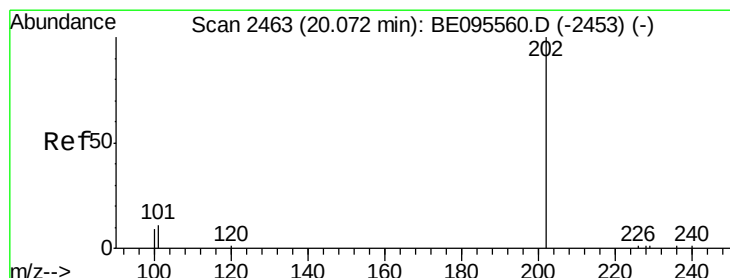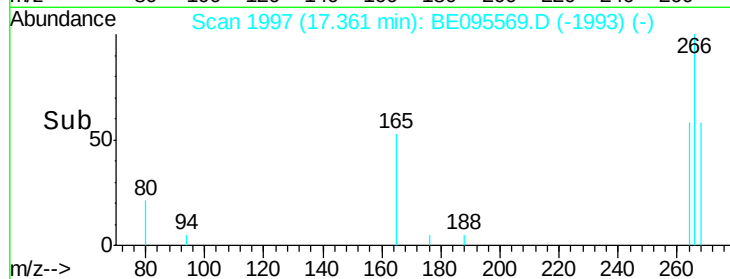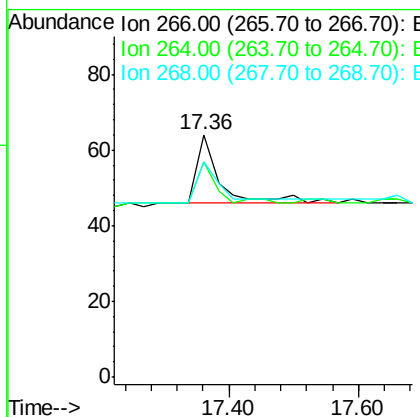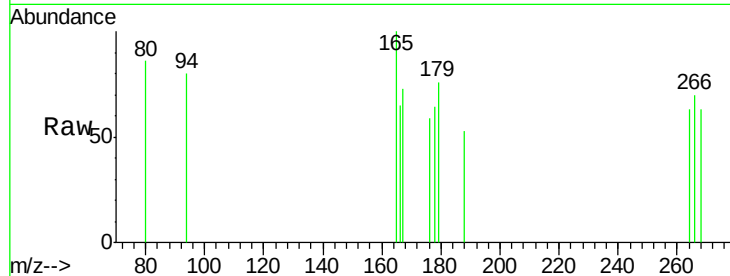

#17
 Pyrene
 Concen: 0.078 ng/ul
 RT: 20.05 min Scan# 2459
 Delta R.T. -0.03 min
 Lab File: BE095569.D
 Acq: 8 Feb 2018 15:07

Tgt Ion:202 Resp: 1716
 Ion Ratio Lower Upper
 202 100
 101 170.4 18.2 27.4#
 100 1191.6 15.6 23.4#

