

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
 Data File : BE095582.D
 Acq On : 8 Feb 2018 22:53
 Operator : SJ/JU
 Sample : J1316-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 09 01:49:03 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 09 01:31:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1718	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4847	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3149	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7253	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7251	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	322981	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2312	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6553	0.24	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	17.36	266	1822	1.297	ng/ul	98
12) Phenanthrene	17.75	178	1994	0.082	ng/ul#	94
15) Fluoranthene	19.72	202	2027	0.064	ng/ul	85
17) Pyrene	20.07	202	3069	0.126	ng/ul#	88
18) Benzo(a)anthracene	21.78	228	495	0.022	ng/ul#	78
19) Chrysene	21.84	228	582	0.025	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
Data File : BE095582.D
Acq On : 8 Feb 2018 22:53
Operator : SJ/JU
Sample : J1316-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 09 01:49:03 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 01:31:22 2018
Response via : Initial Calibration

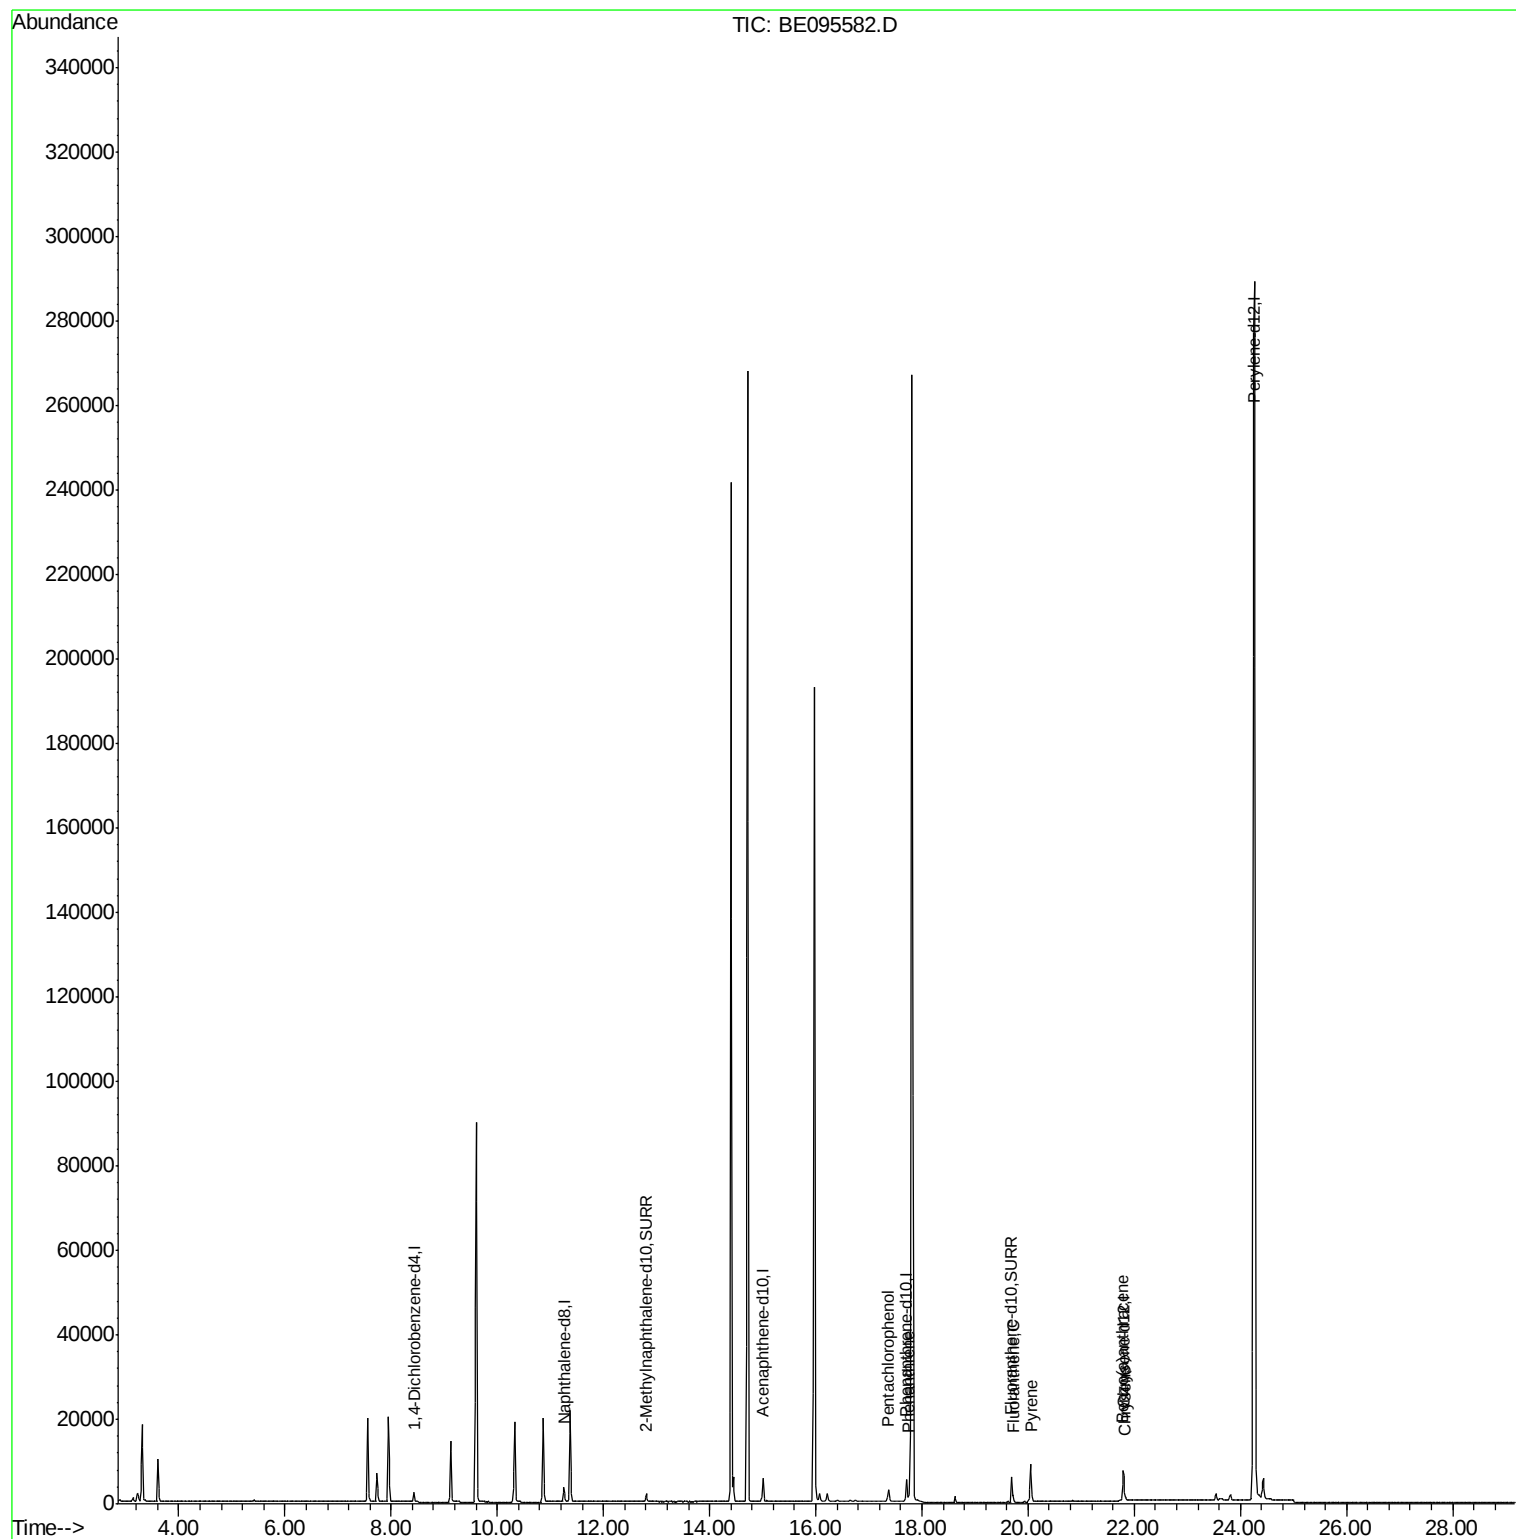


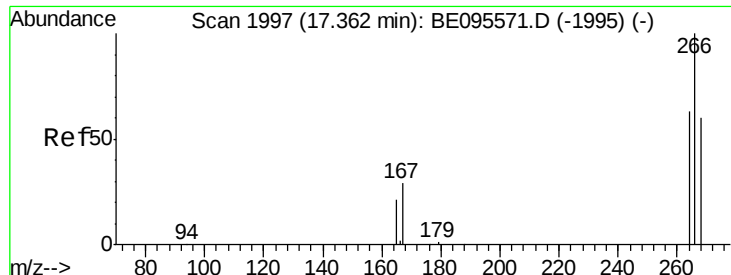




#11
 Pentachlorophenol
 Concen: 1.297 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095582.D
 Acq: 8 Feb 2018 22:53

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:266 Resp: 1822
 Ion Ratio Lower Upper
 266 100
 264 62.2 47.9 71.9
 268 62.7 49.8 74.8

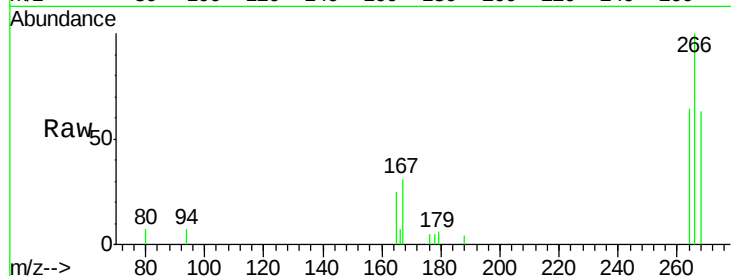


Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

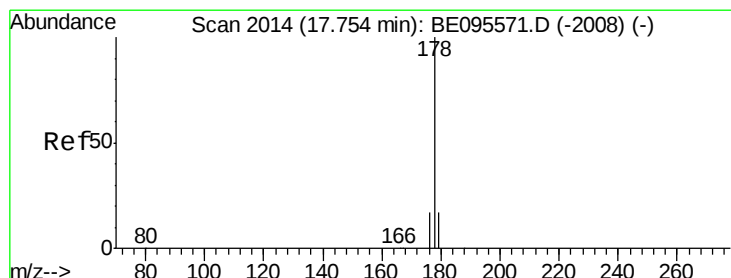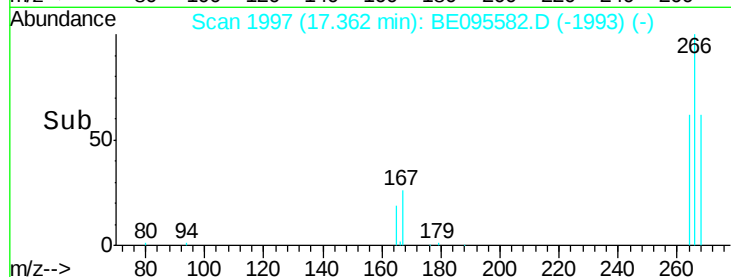
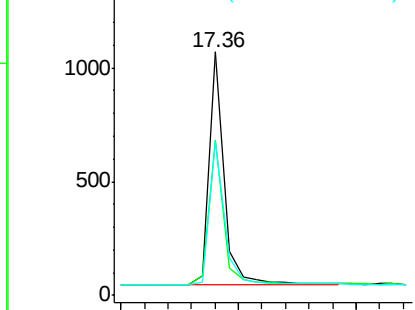



#12
 Phenanthrene
 Concen: 0.082 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. -0.00 min
 Lab File: BE095582.D
 Acq: 8 Feb 2018 22:53

Tgt Ion:178 Resp: 1994
 Ion Ratio Lower Upper
 178 100
 179 21.7 18.4 27.6
 176 21.0 13.6 20.4#

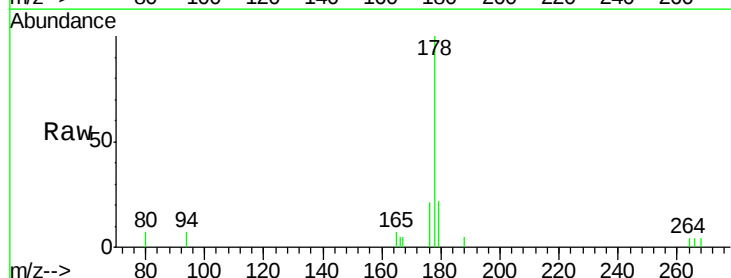

Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

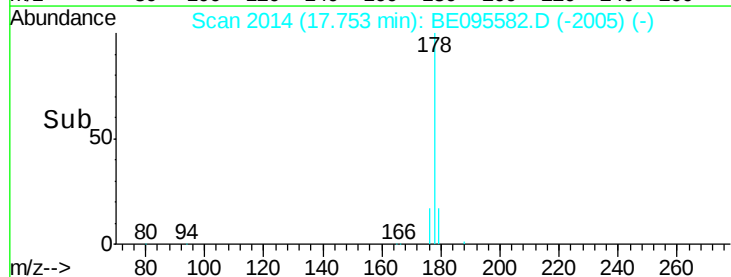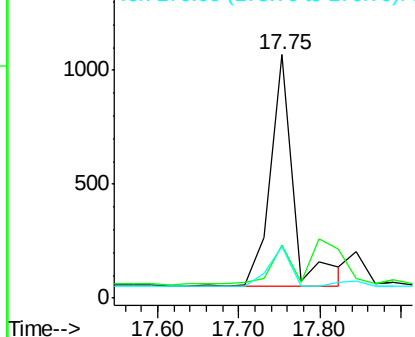

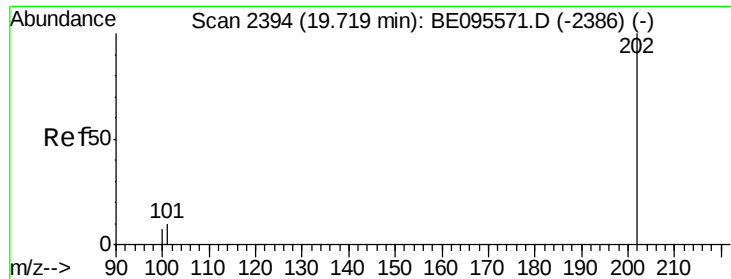

#15

Fluoranthene

Concen: 0.064 ng/ul

RT: 19.72 min Scan# 2394

Delta R.T. 0.00 min

Lab File: BE095582.D

Acq: 8 Feb 2018 22:53

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 2027

Ion Ratio Lower Upper

202 100

101 12.5 0.0 30.3




100 10.2 0.0 39.5

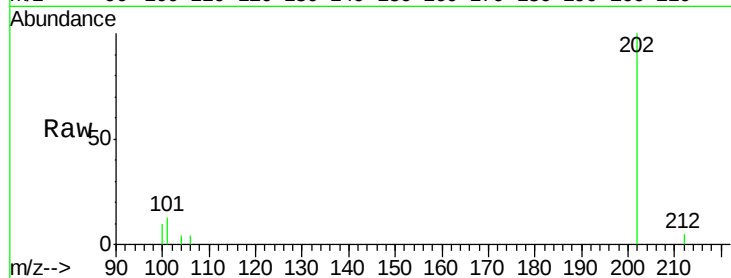

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

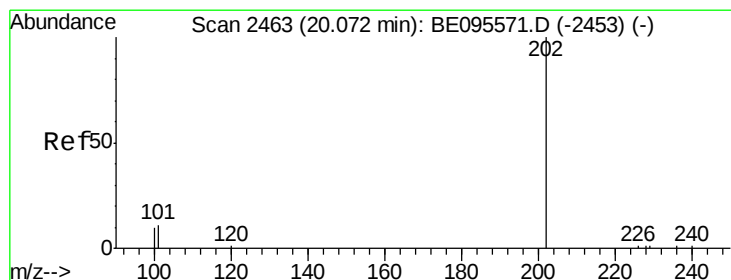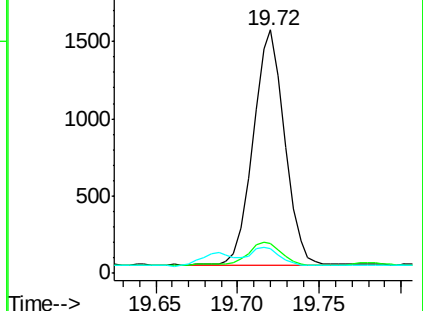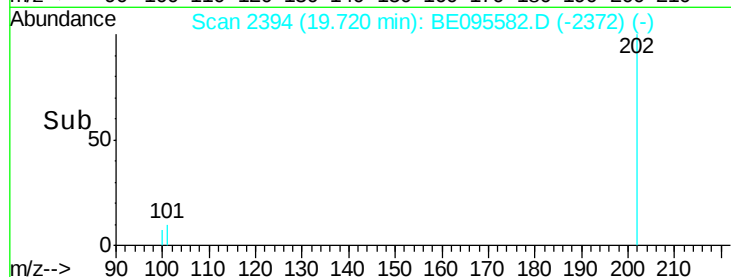

#17

Pyrene

Concen: 0.126 ng/ul

RT: 20.07 min Scan# 2463

Delta R.T. -0.00 min

Lab File: BE095582.D

Acq: 8 Feb 2018 22:53


Tgt Ion:202 Resp: 3069

Ion Ratio Lower Upper

202 100

101 15.0 18.2 27.4#



100 16.4 15.6 23.4

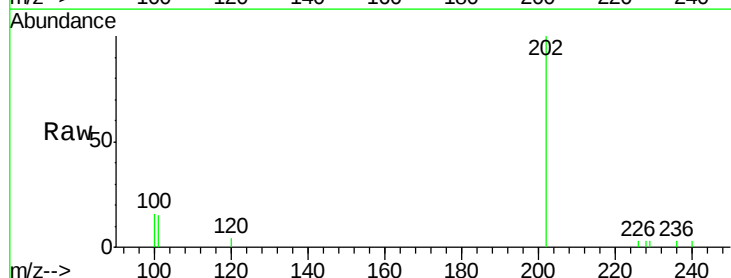


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

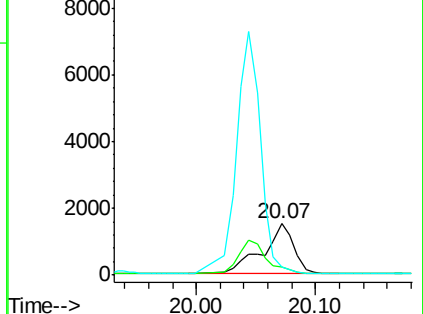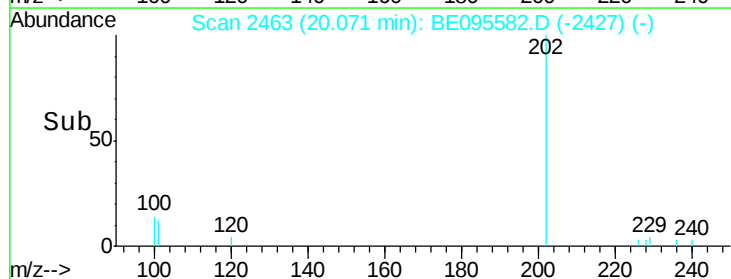

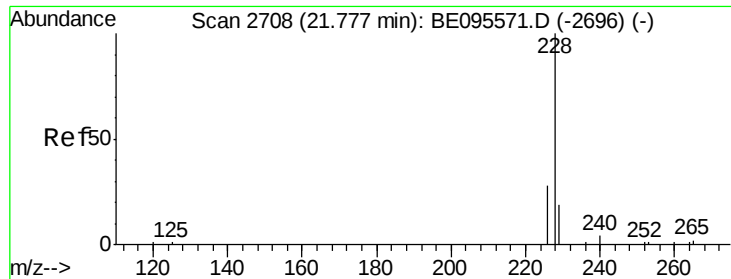

#18

Benzo(a)anthracene

Concen: 0.022 ng/ul

RT: 21.78 min Scan# 2709

Delta R.T. 0.00 min

Lab File: BE095582.D

Acq: 8 Feb 2018 22:53

Instrument :

BNA_E

ClientSampleId :





Tot Ion:228 Resp: 495

Ion Ratio Lower Upper

228 100

229 34.6 22.8 34.2#

226 38.0 17.0 25.6#

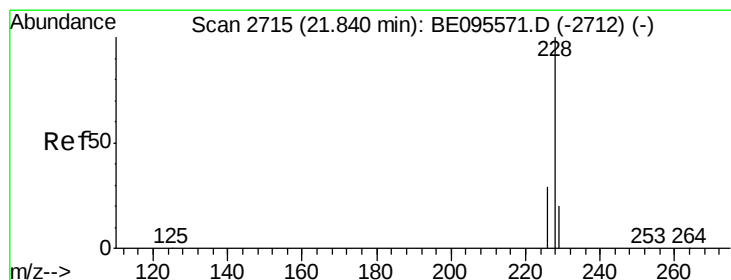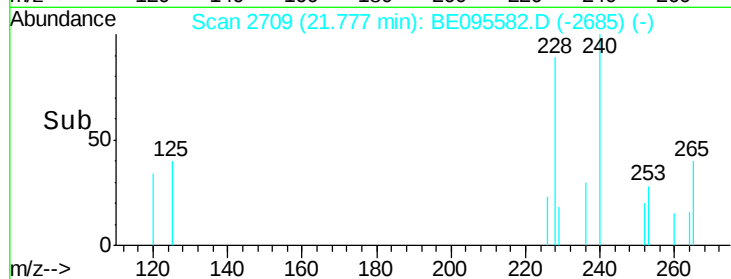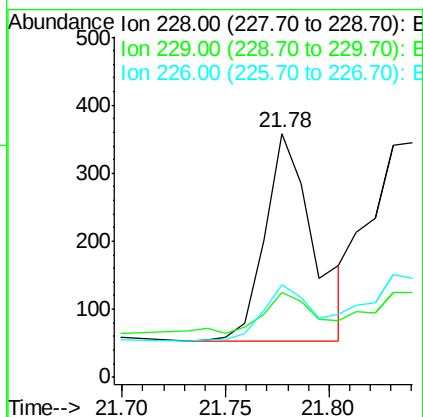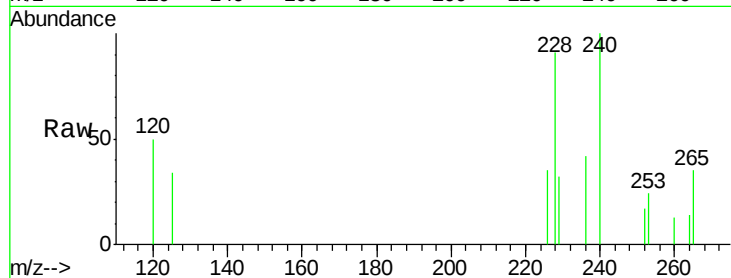

#19

Chrysene

Concen: 0.025 ng/ul

RT: 21.84 min Scan# 2716

Delta R.T. 0.00 min

Lab File: BE095582.D

Acq: 8 Feb 2018 22:53

Tgt Ion:228 Resp: 582

Ion Ratio Lower Upper

228 100

226 42.0 23.4 35.0#

229 36.2 17.7 26.5#

