

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
 Data File : BE095583.D
 Acq On : 8 Feb 2018 23:29
 Operator : SJ/JU
 Sample : J1316-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 09 01:49:11 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 09 01:31:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1853	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5322	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3506	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8431	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7918	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	367364	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2510	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7170	0.22	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	668	0.409	ng/ul	99
17) Pyrene	20.04	202	1149	0.043	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
Data File : BE095583.D
Acq On : 8 Feb 2018 23:29
Operator : SJ/JU
Sample : J1316-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 09 01:49:11 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 01:31:22 2018
Response via : Initial Calibration

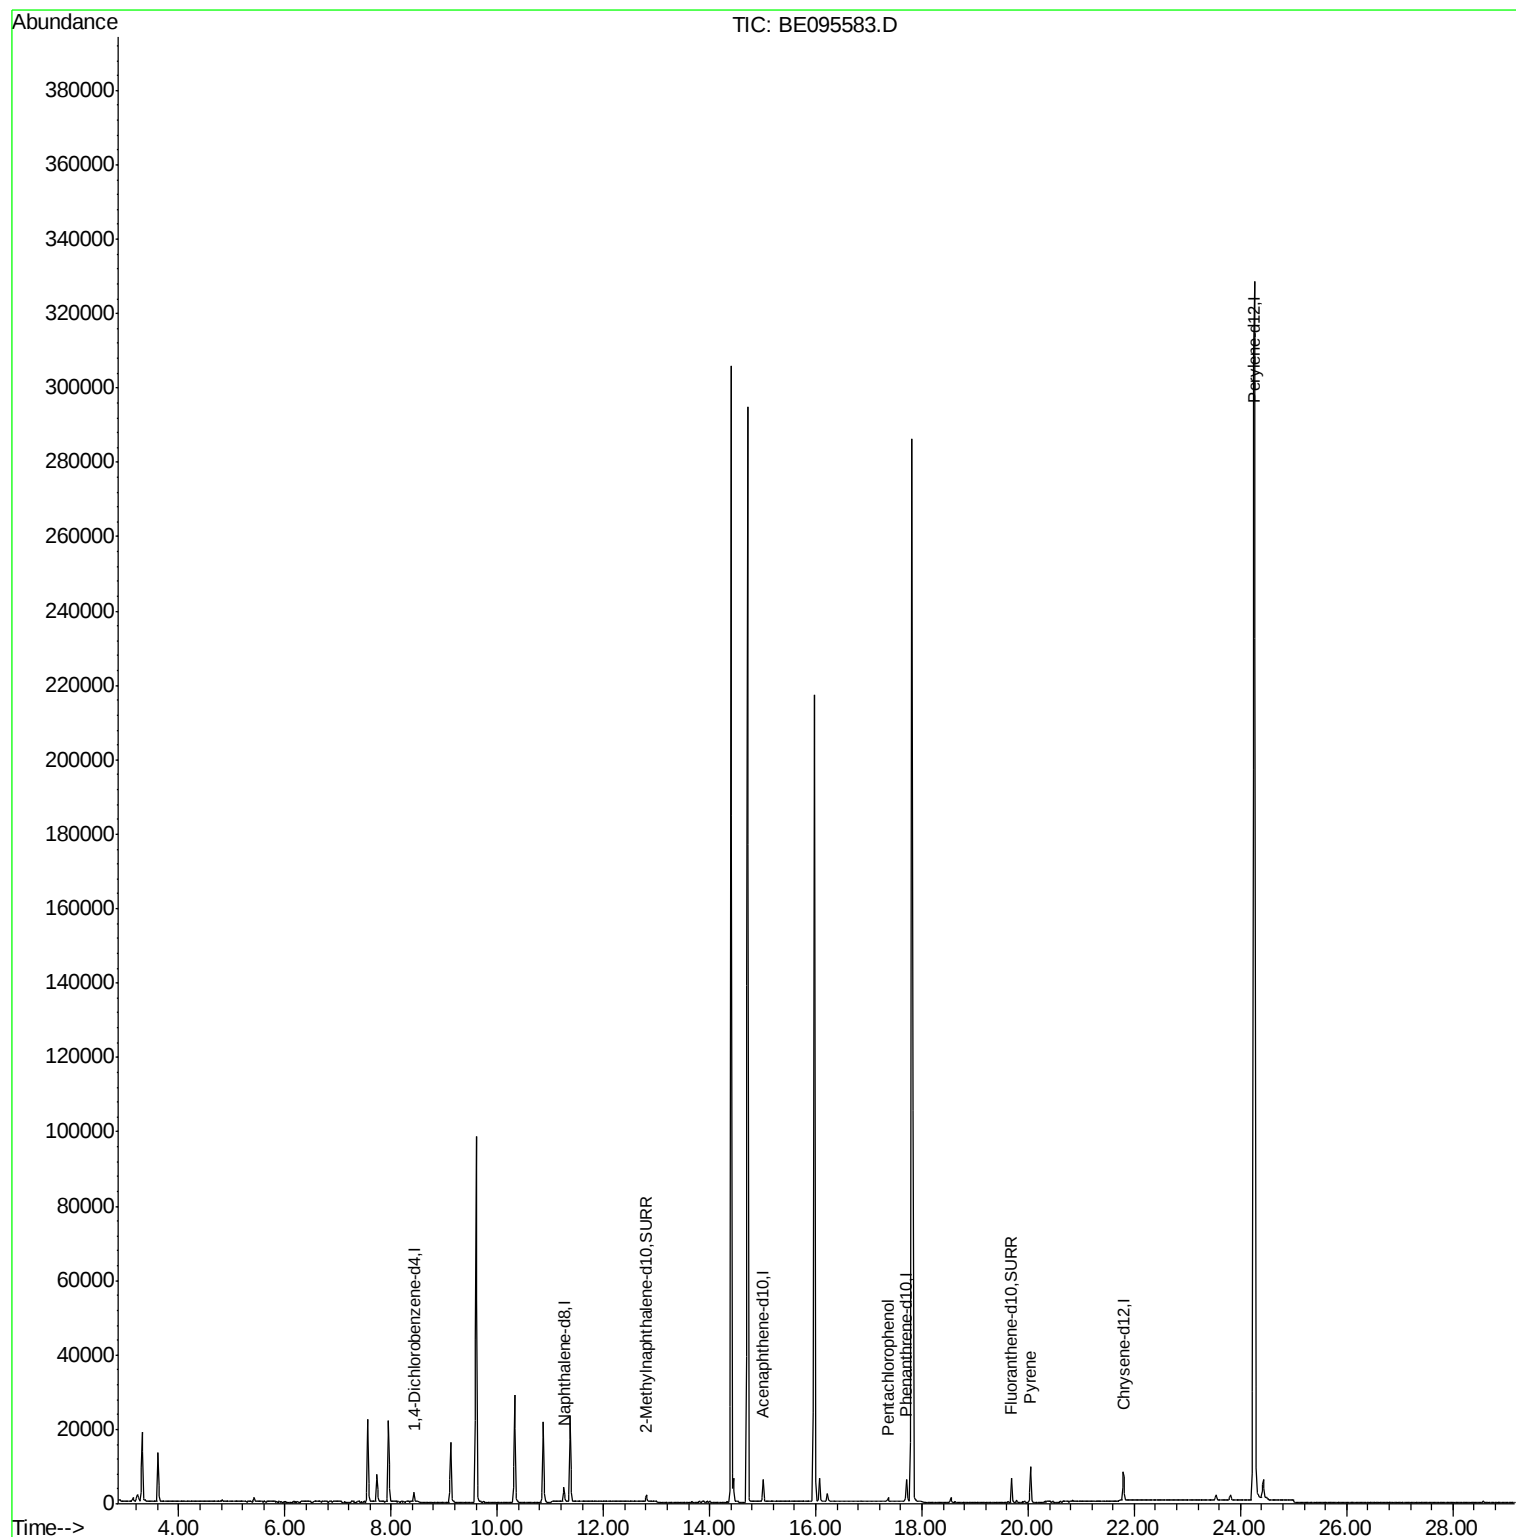


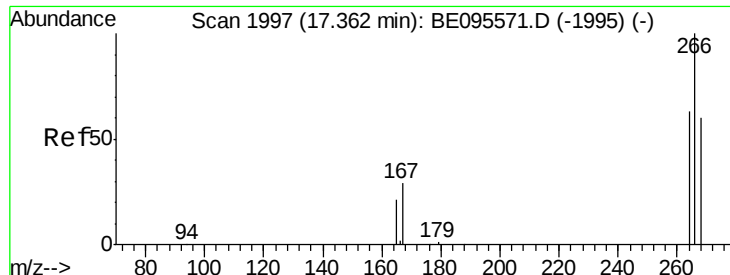




#11
 Pentachlorophenol
 Concen: 0.409 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095583.D
 Acq: 8 Feb 2018 23:29

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:266 Resp: 668
 Ion Ratio Lower Upper
 266 100
 264 61.2 47.9 71.9
 268 62.7 49.8 74.8

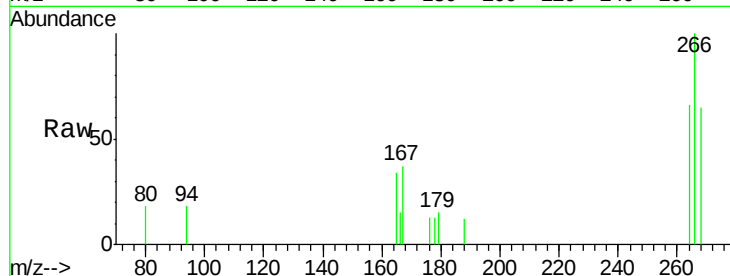


Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

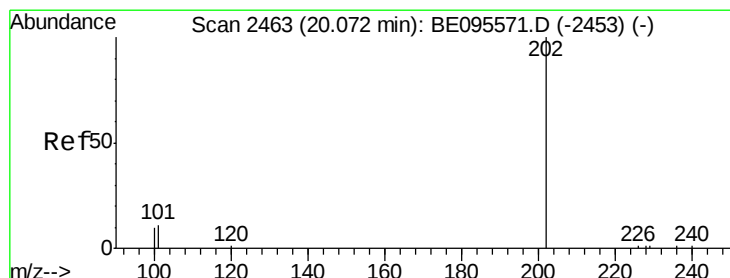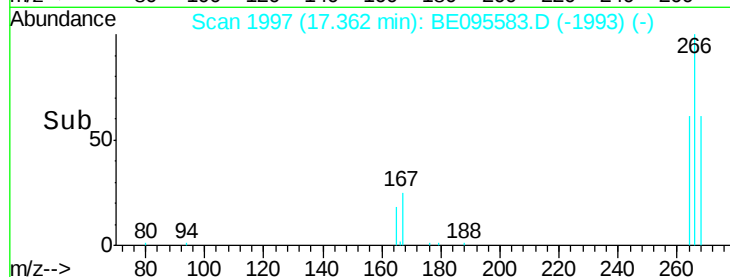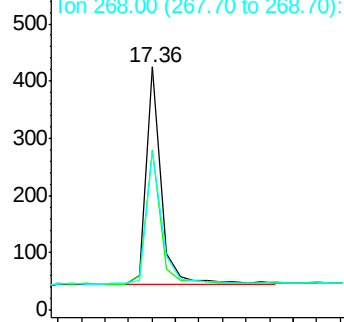

#17
 Pyrene
 Concen: 0.043 ng/ul
 RT: 20.04 min Scan# 2459
 Delta R.T. -0.03 min
 Lab File: BE095583.D
 Acq: 8 Feb 2018 23:29

Tgt Ion:202 Resp: 1149
 Ion Ratio Lower Upper
 202 100
 101 168.5 18.2 27.4#
 100 1180.9 15.6 23.4#

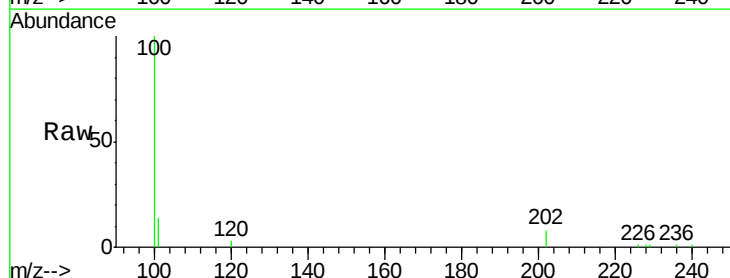

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): E

