

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
 Data File : BE095584.D
 Acq On : 9 Feb 2018 00:05
 Operator : SJ/JU
 Sample : J1316-20
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 09 04:07:13 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 09 01:31:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1764	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4922	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3274	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7382	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7516	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	504096	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3127	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9355	0.33	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	29	0.020	ng/ul#	70
17) Pyrene	20.05	202	1423	0.056	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
Data File : BE095584.D
Acq On : 9 Feb 2018 00:05
Operator : SJ/JU
Sample : J1316-20
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 09 04:07:13 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 01:31:22 2018
Response via : Initial Calibration




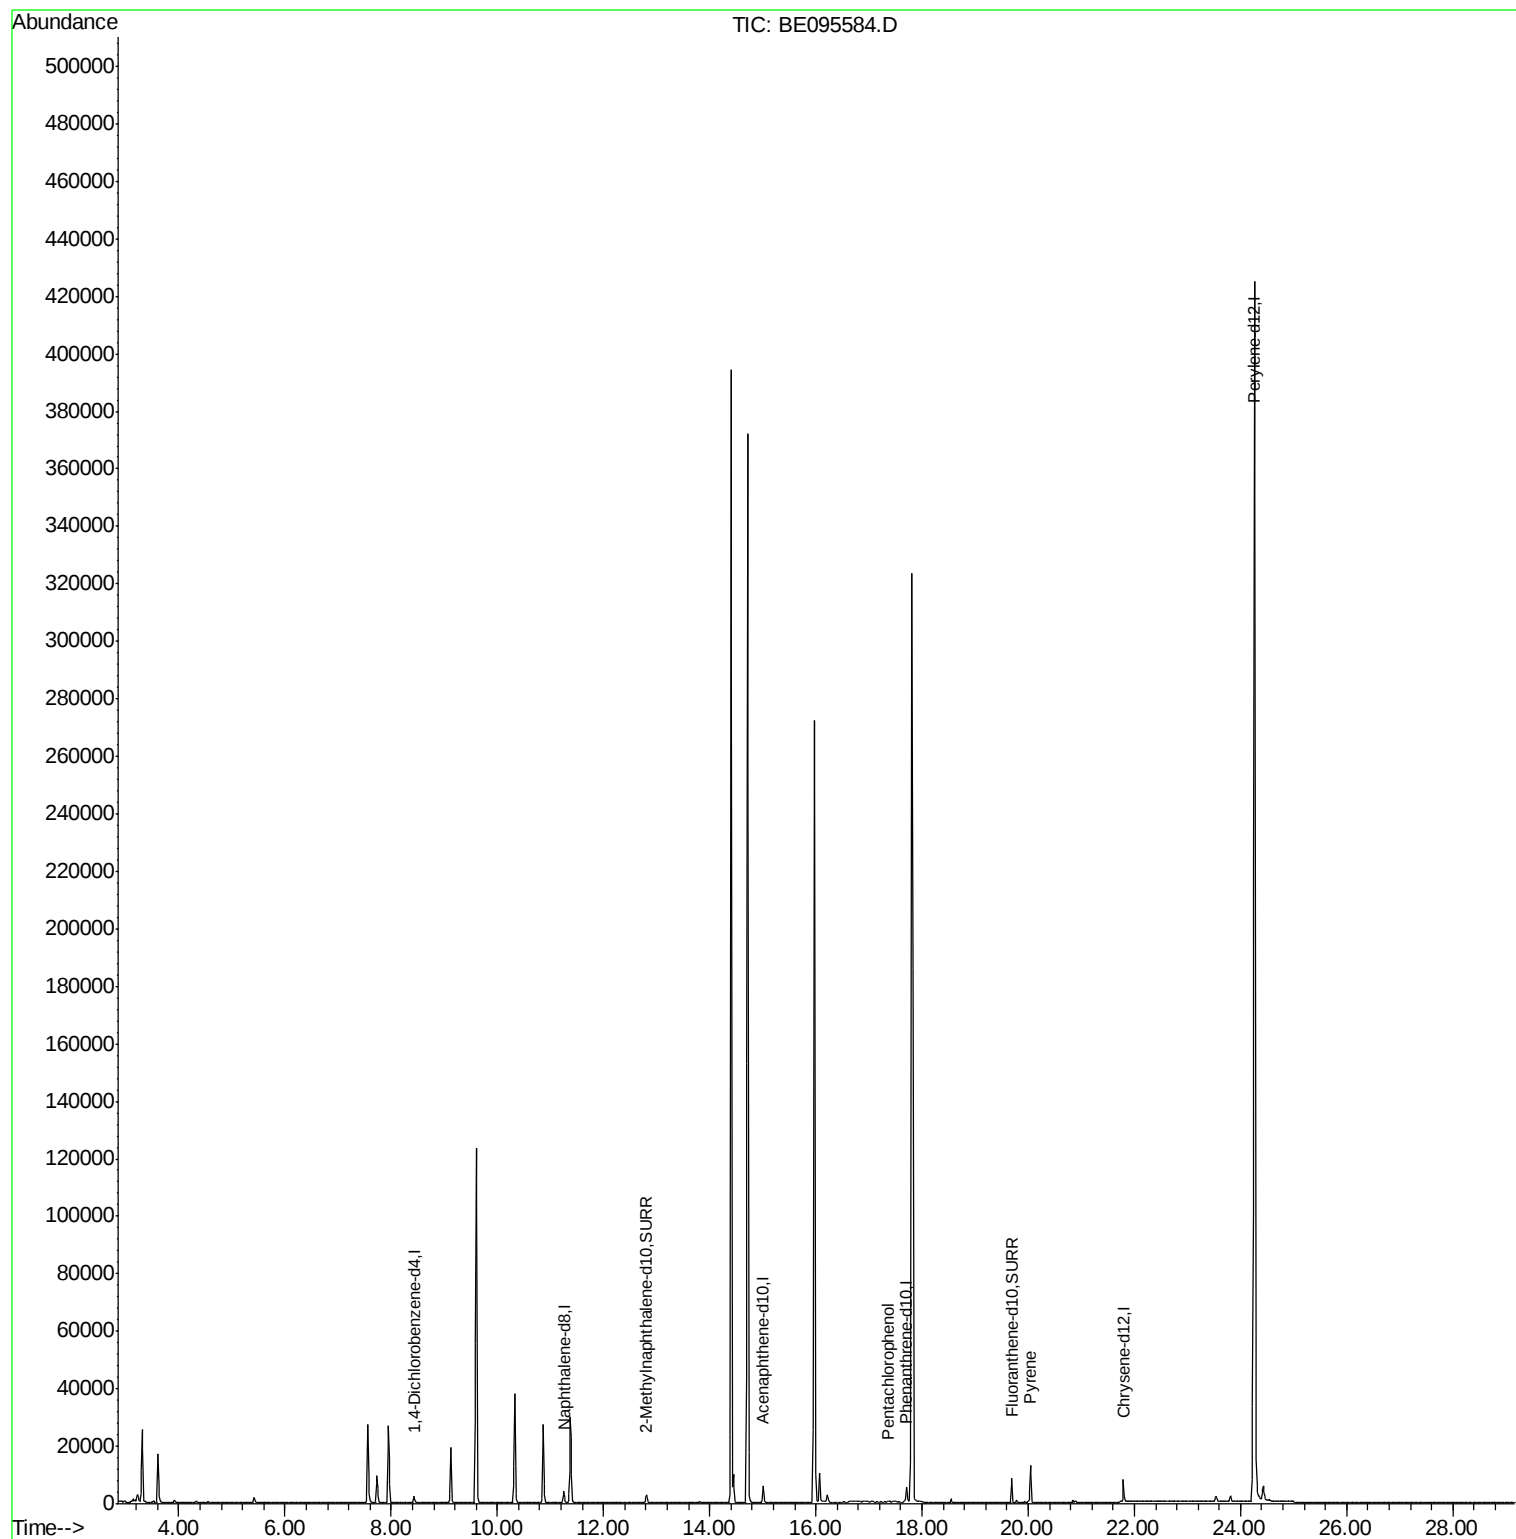


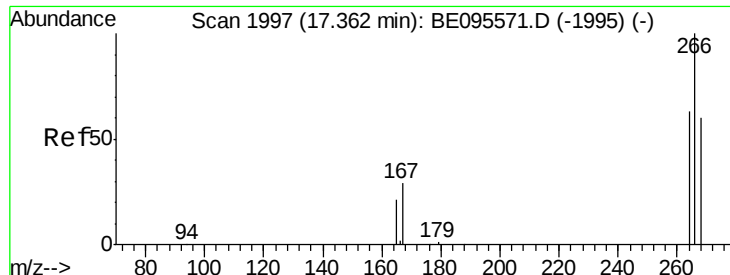

#11
 Pentachlorophenol
 Concen: 0.020 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095584.D
 Acq: 9 Feb 2018 00:05

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
266	100		
264	48.3	47.9	71.9
268	96.6	49.8	74.8#

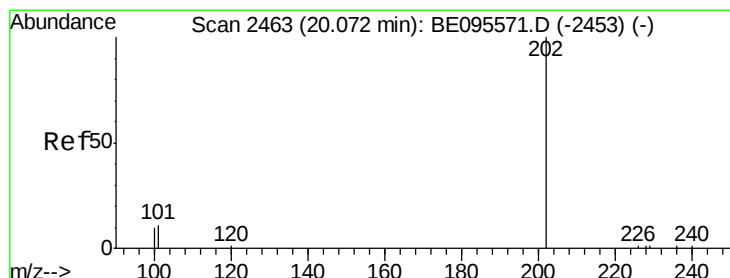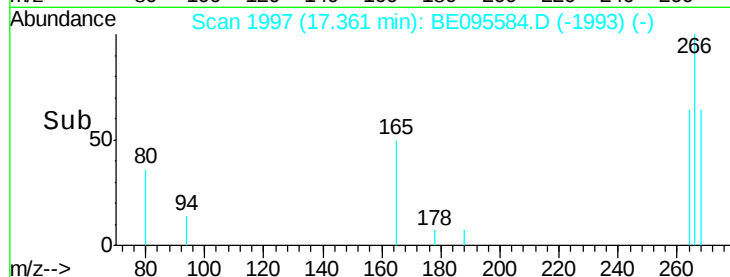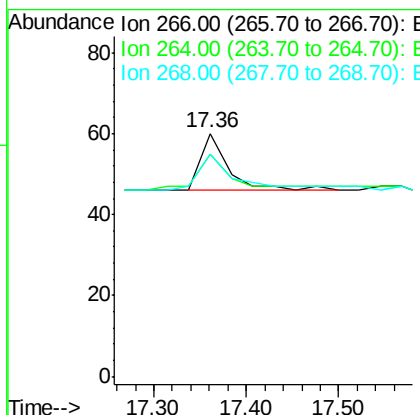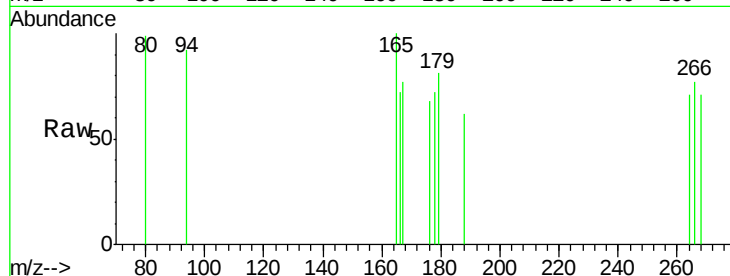

#17
 Pyrene
 Concen: 0.056 ng/ul
 RT: 20.05 min Scan# 2459
 Delta R.T. -0.03 min
 Lab File: BE095584.D
 Acq: 9 Feb 2018 00:05

Tgt Ion	Ratio	Lower	Upper
202	100		
101	177.2	18.2	27.4#
100	1255.0	15.6	23.4#

