

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
 Data File : BE095587.D
 Acq On : 9 Feb 2018 2:46
 Operator : SJ/JU
 Sample : J1317-14
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 09 04:49:01 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 09 04:15:12 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.42	152	1911	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5390	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3441	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8183	0.40	ng/ul	0.00
16) Chrysene-d12	21.79	240	7805	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	450280	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2913	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7990	0.26	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	17.36	266	44	0.028	ng/ul	94
12) Phenanthrene	17.75	178	704	0.026	ng/ul#	66
17) Pyrene	20.04	202	1520	0.058	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
Data File : BE095587.D
Acq On : 9 Feb 2018 2:46
Operator : SJ/JU
Sample : J1317-14
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 09 04:49:01 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 04:15:12 2018
Response via : Initial Calibration




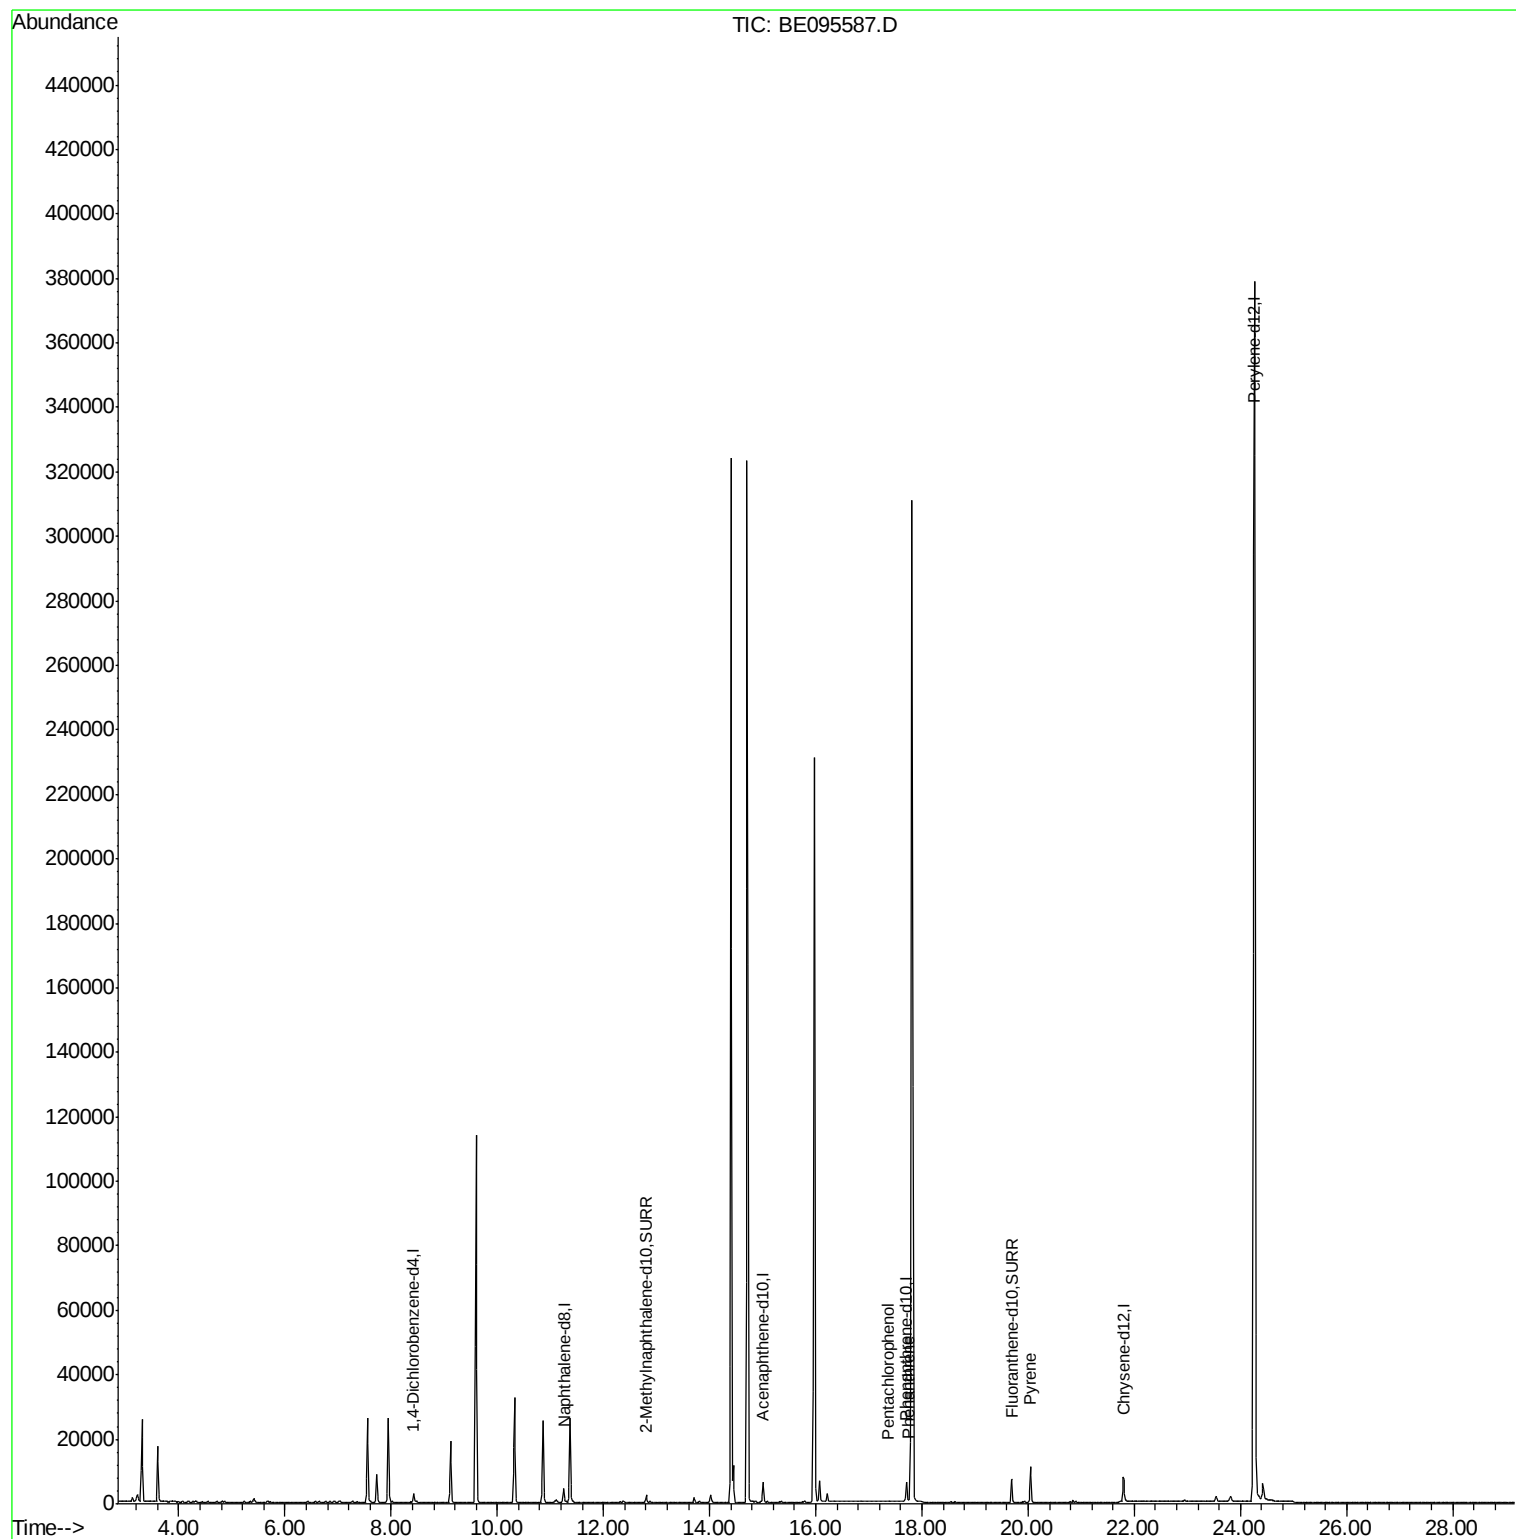


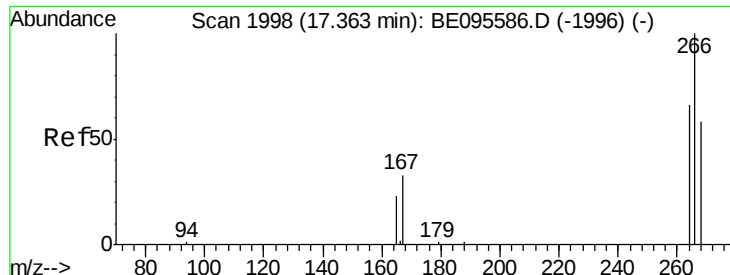

#11
 Pentachlorophenol
 Concen: 0.028 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095587.D
 Acq: 9 Feb 2018 2:46




Instrument :
 BNA_E
 ClientSampled :


Tot Ion:266 Resp: 44
 Ion Ratio Lower Upper
 266 100
 264 68.2 47.9 71.9
 268 63.6 49.8 74.8

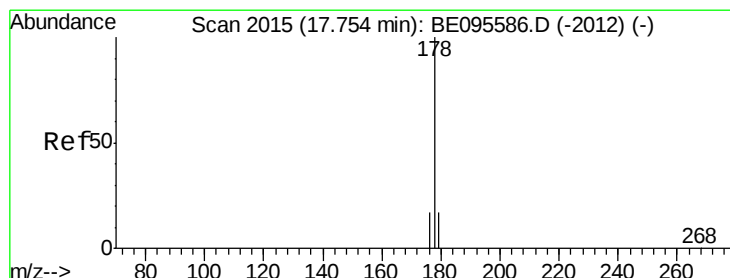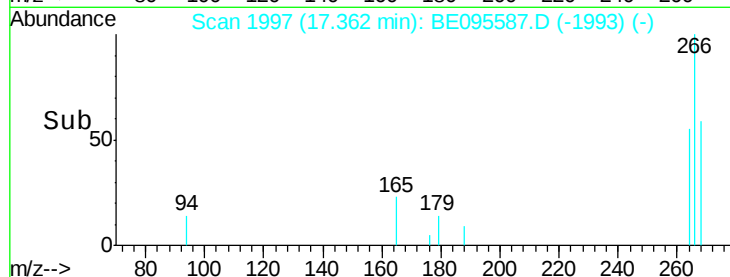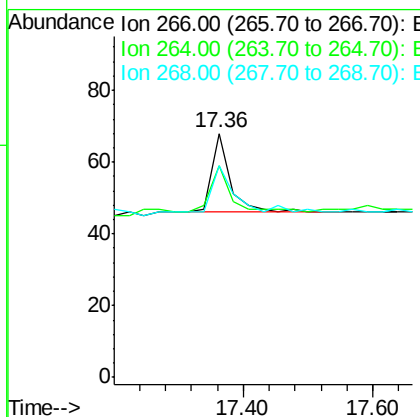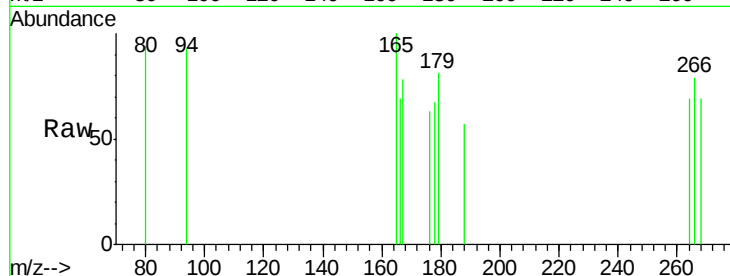

#12
 Phenanthrene
 Concen: 0.026 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. -0.00 min
 Lab File: BE095587.D
 Acq: 9 Feb 2018 2:46

Tgt Ion:178 Resp: 704
 Ion Ratio Lower Upper
 178 100
 179 38.2 18.4 27.6#
 176 33.8 13.6 20.4#

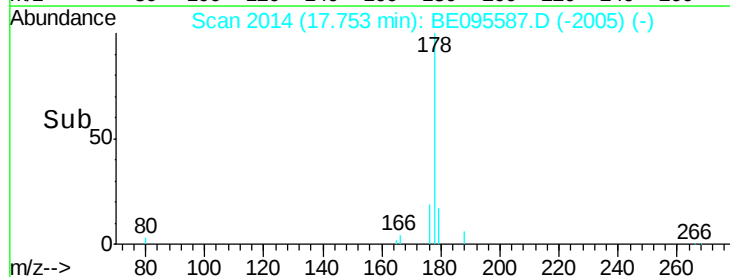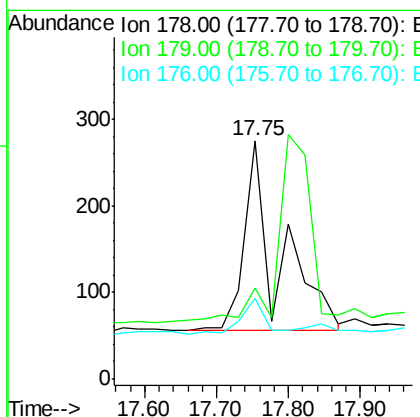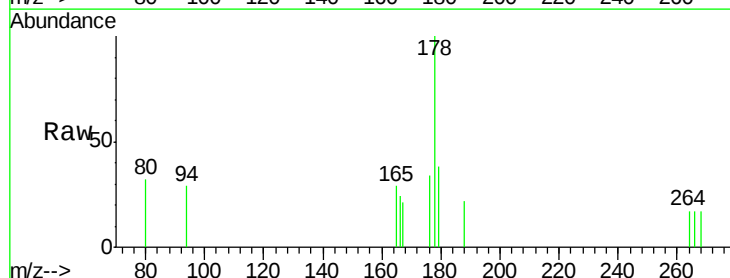

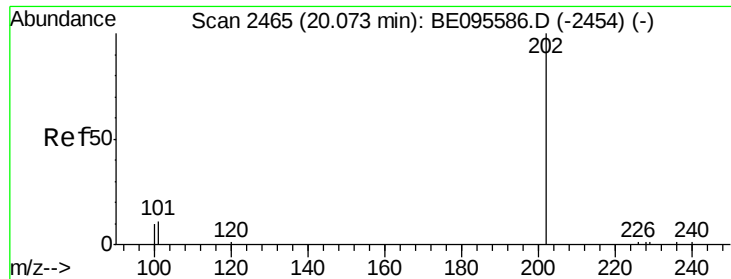

#17
 Pvrene
 Concen: 0.058 ng/ul
 RT: 20.04 min Scan# 2459
 Delta R.T. -0.03 min
 Lab File: BE095587.D
 Acq: 9 Feb 2018 2:46

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion: 202 Resp: 1520
 Ion Ratio Lower Upper
 202 100
 101 168.2 18.2 27.4#
 100 1171.5 15.6 23.4#

