

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
 Data File : BE095588.D
 Acq On : 9 Feb 2018 3:22
 Operator : SJ/JU
 Sample : J1317-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 09 04:49:06 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 09 04:15:12 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1844	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5386	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3539	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8172	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7907	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	500518	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3301	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9413	0.30	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	278	0.176	ng/ul	100
12) Phenanthrene	17.75	178	1087	0.040	ng/ul#	78
17) Pyrene	20.05	202	1750	0.066	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
Data File : BE095588.D
Acq On : 9 Feb 2018 3:22
Operator : SJ/JU
Sample : J1317-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 09 04:49:06 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 04:15:12 2018
Response via : Initial Calibration




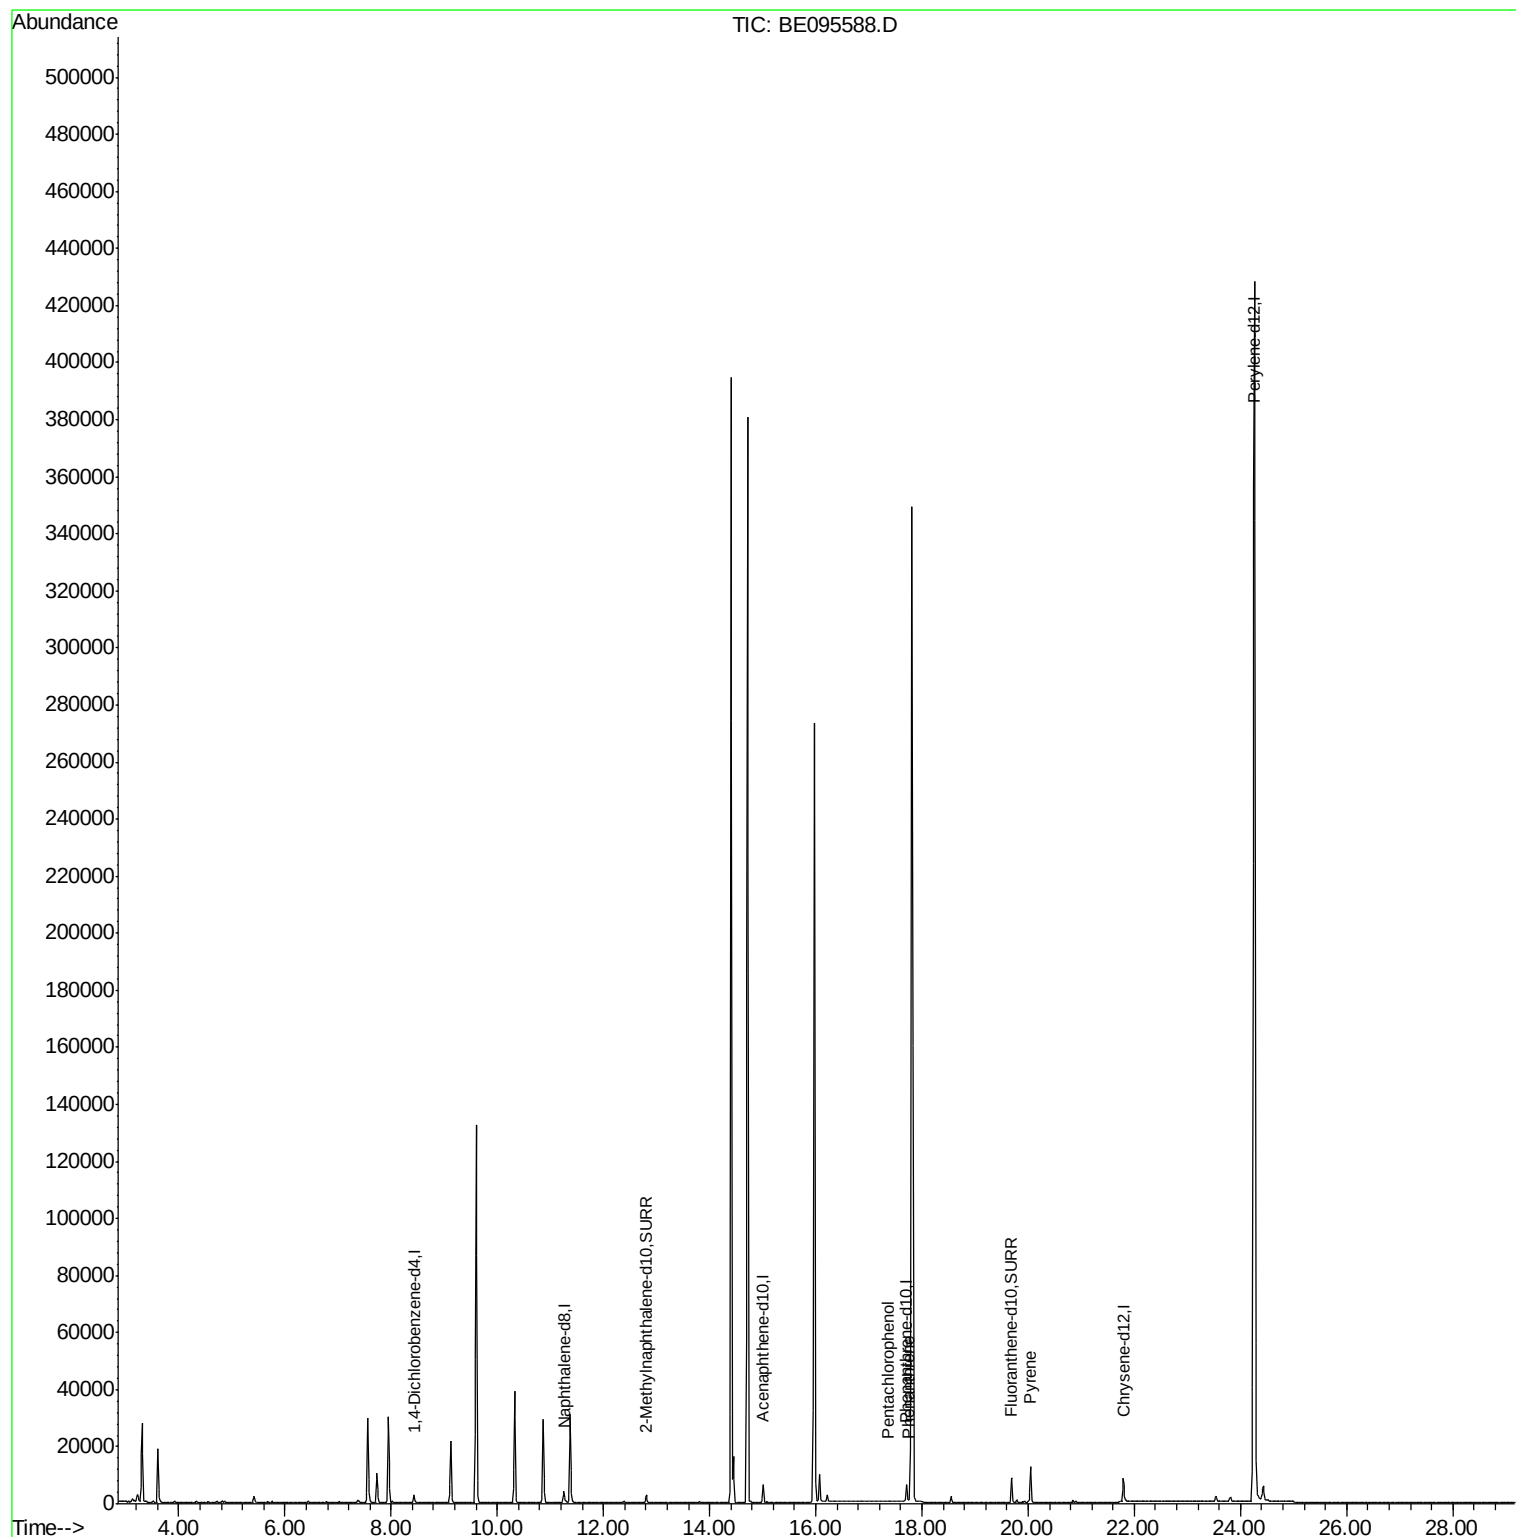


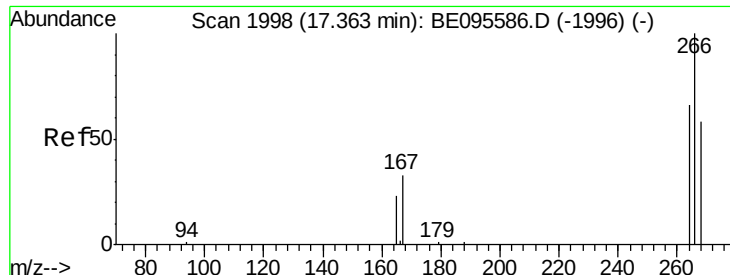

#11
 Pentachlorophenol
 Concen: 0.176 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095588.D
 Acq: 9 Feb 2018 3:22




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 278
 Ion Ratio Lower Upper
 266 100
 264 59.7 47.9 71.9
 268 62.6 49.8 74.8

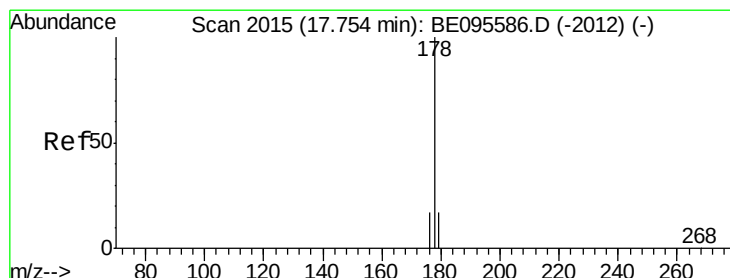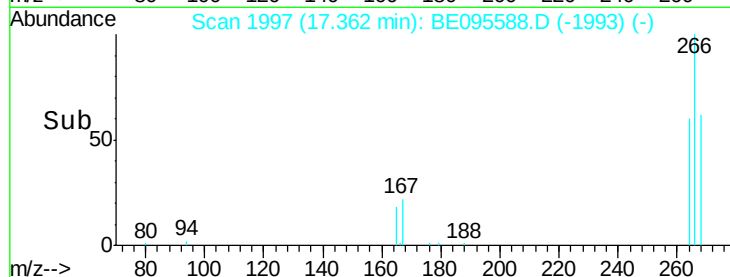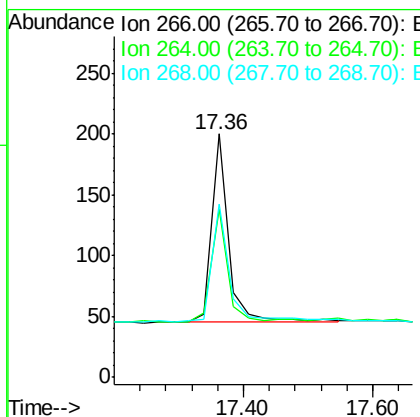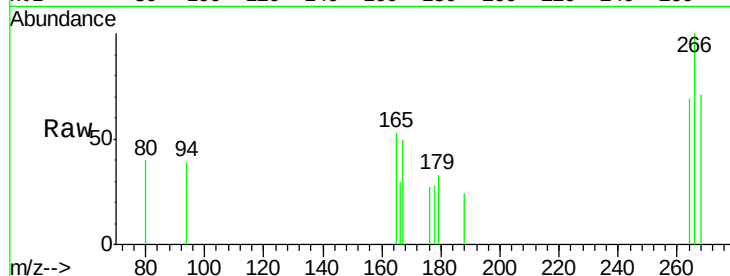

#12
 Phenanthrene
 Concen: 0.040 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. -0.00 min
 Lab File: BE095588.D
 Acq: 9 Feb 2018 3:22

Tgt Ion:178 Resp: 1087
 Ion Ratio Lower Upper
 178 100
 179 31.0 18.4 27.6#
 176 29.2 13.6 20.4#

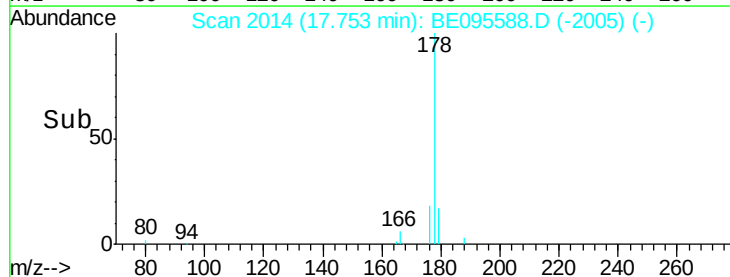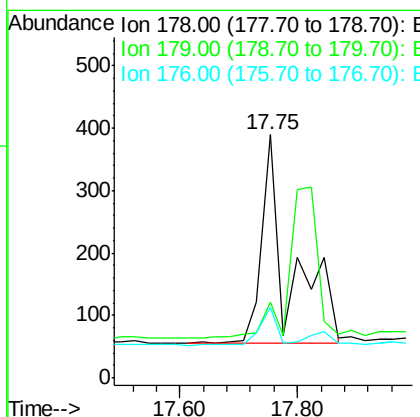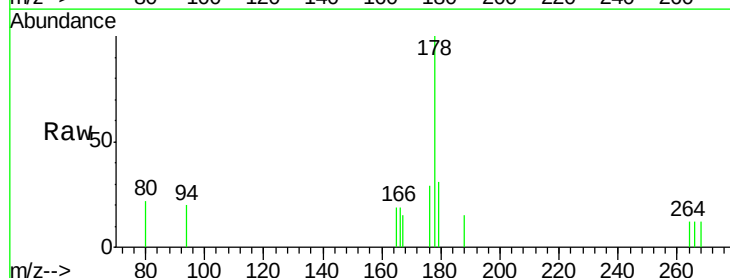

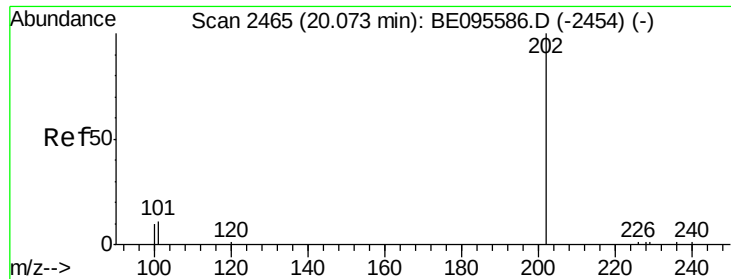

#17
 Pvrene
 Concen: 0.066 ng/ul
 RT: 20.05 min Scan# 2460
 Delta R.T. -0.02 min
 Lab File: BE095588.D
 Acq: 9 Feb 2018 3:22

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
202	100		
101	155.7	18.2	27.4#
100	972.4	15.6	23.4#

