

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095564.D

Acq On : 8 Feb 2018 12:08

Operator : SJ/JU

Sample : J1316-18

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: Feb 09 00:47:05 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 00:43:28 2018

Response via : Initial Calibration

Instrument :

BNA_E




ClientSampleId :

F6C98

Manual Integrations
APPROVED

Sohil

2/9/2018 4:30:27 PM

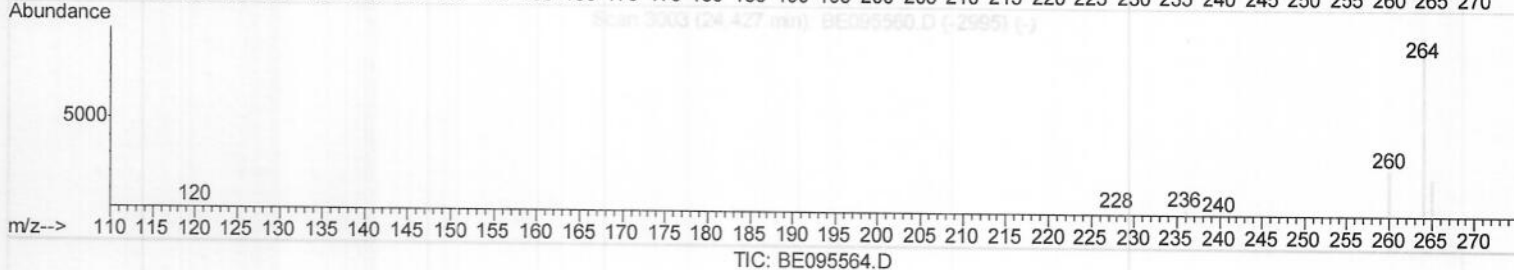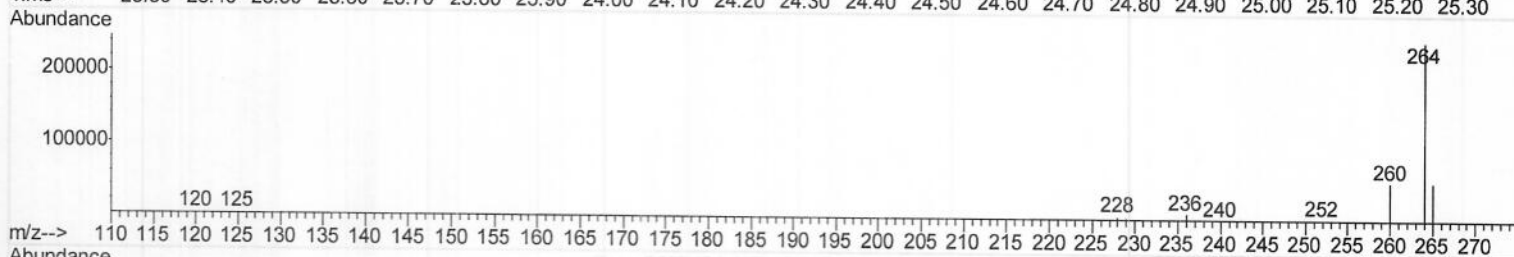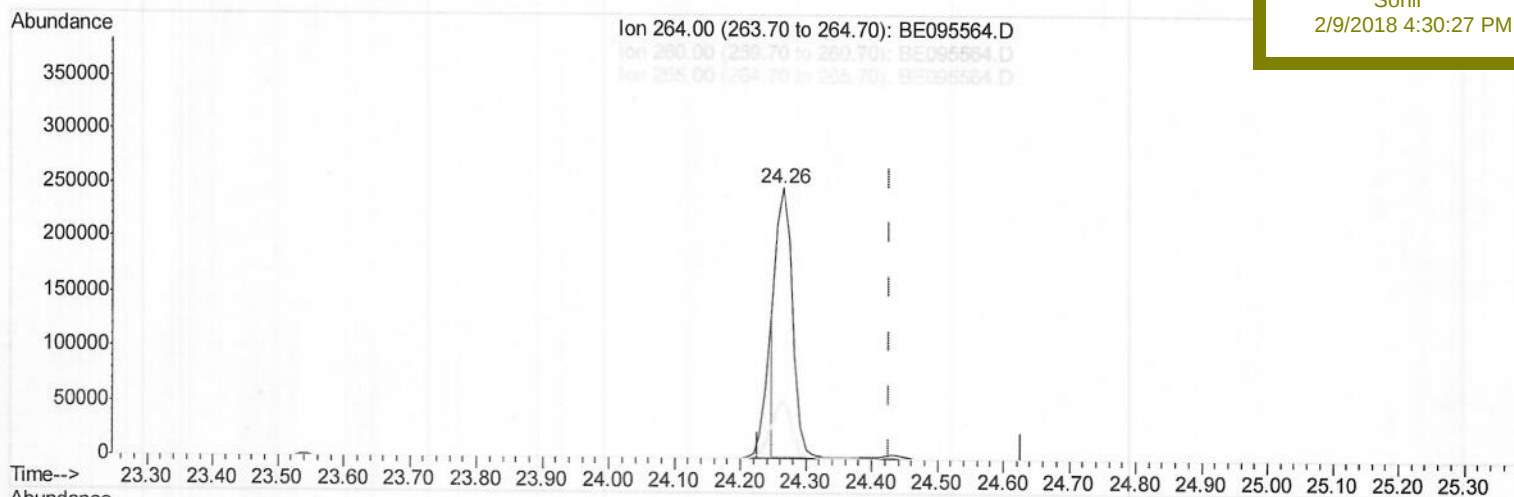

(20) Perylene-d12 (I)

24.265min (-0.162) 0.40ng/ui

response 426891

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.19#
265.00	103.50	21.41#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095564.D

Acq On : 8 Feb 2018 12:08

Operator : SJ/JU

Sample : J1316-18

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: Feb 09 00:47:05 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 00:43:28 2018

Response via : Initial Calibration

Instrument :

BNA_E



ClientSampleId :

F6C98

Manual Integrations
APPROVED

Sohil

2/9/2018 4:30:27 PM

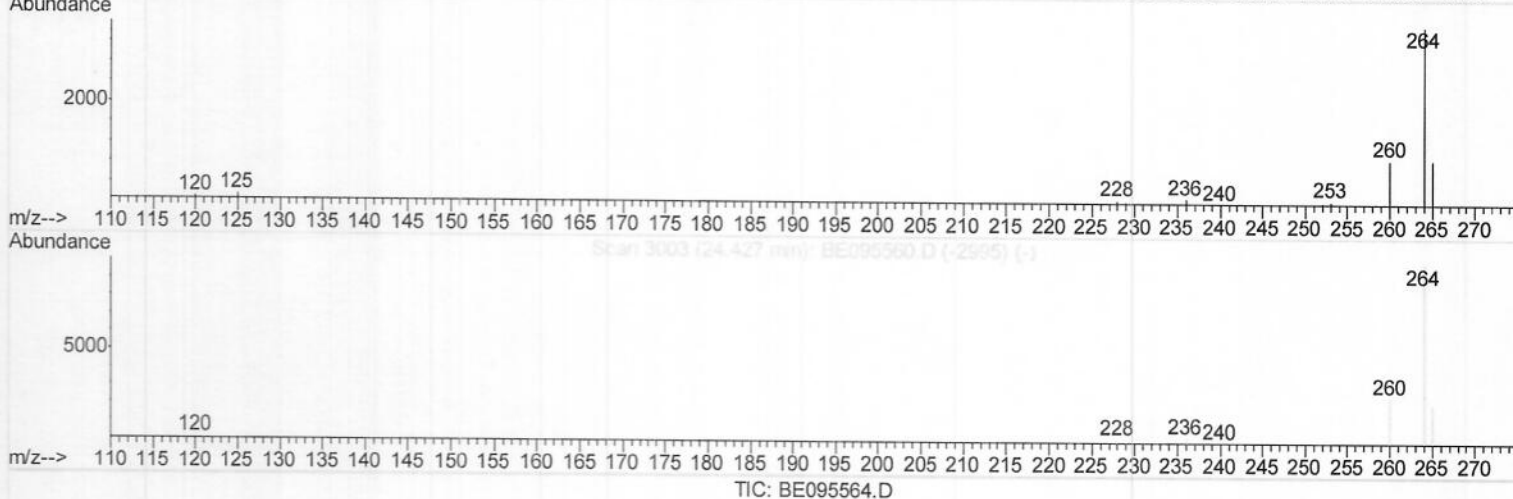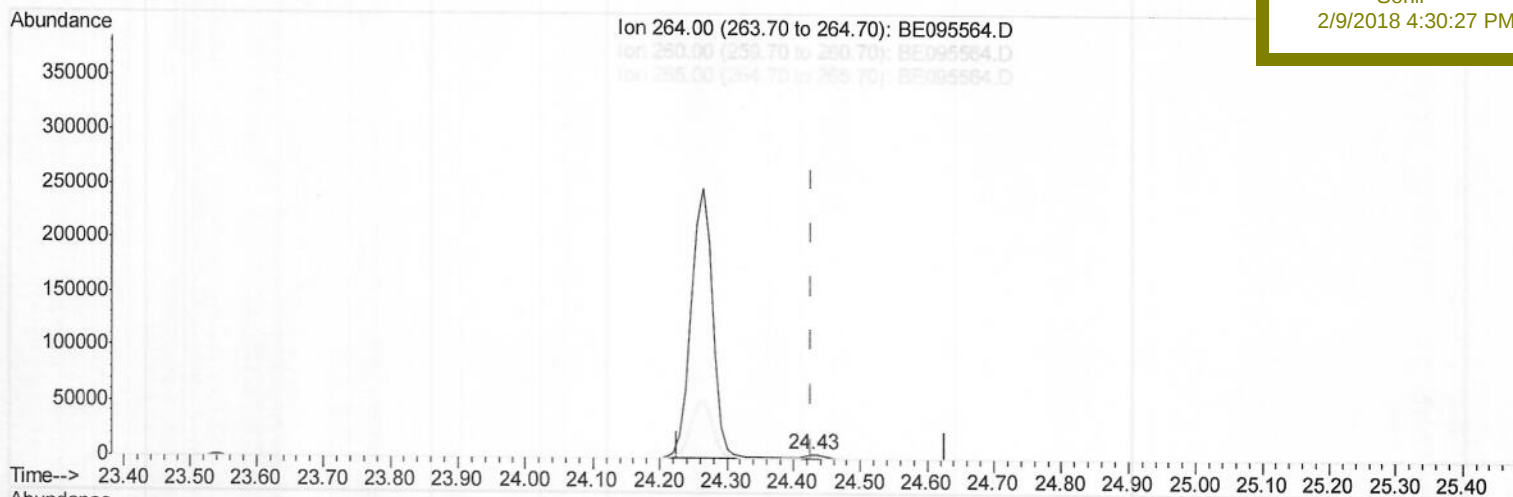

(20) Perylene-d12 (I)

24.427min (+0.000) 0.40ng/ul m S JY02113118

response 6717

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.09
265.00	103.50	25.70#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095564.D

Acq On : 8 Feb 2018 12:08

Operator : SJ/JU

Sample : J1316-18

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: Feb 09 01:09:27 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 00:43:28 2018

Response via : Initial Calibration

Instrument :

BNA_E

Client Sampled :

F6C98

Manual Integrations

APPROVED

Sohil

2/9/2018 4:30:27 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1700	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4685	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3093	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7207	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7451	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	6717m)	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2670	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8037	0.29	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	365	0.261	ng/ul	Ovalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JY 02/13/18

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095564.D

Acq On : 8 Feb 2018 12:08

Operator : SJ/JU

Sample : J1316-18

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: Feb 09 01:09:27 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 00:43:28 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6C98

Manual Integrations

APPROVED

Sohil

2/9/2018 4:30:27 PM

